
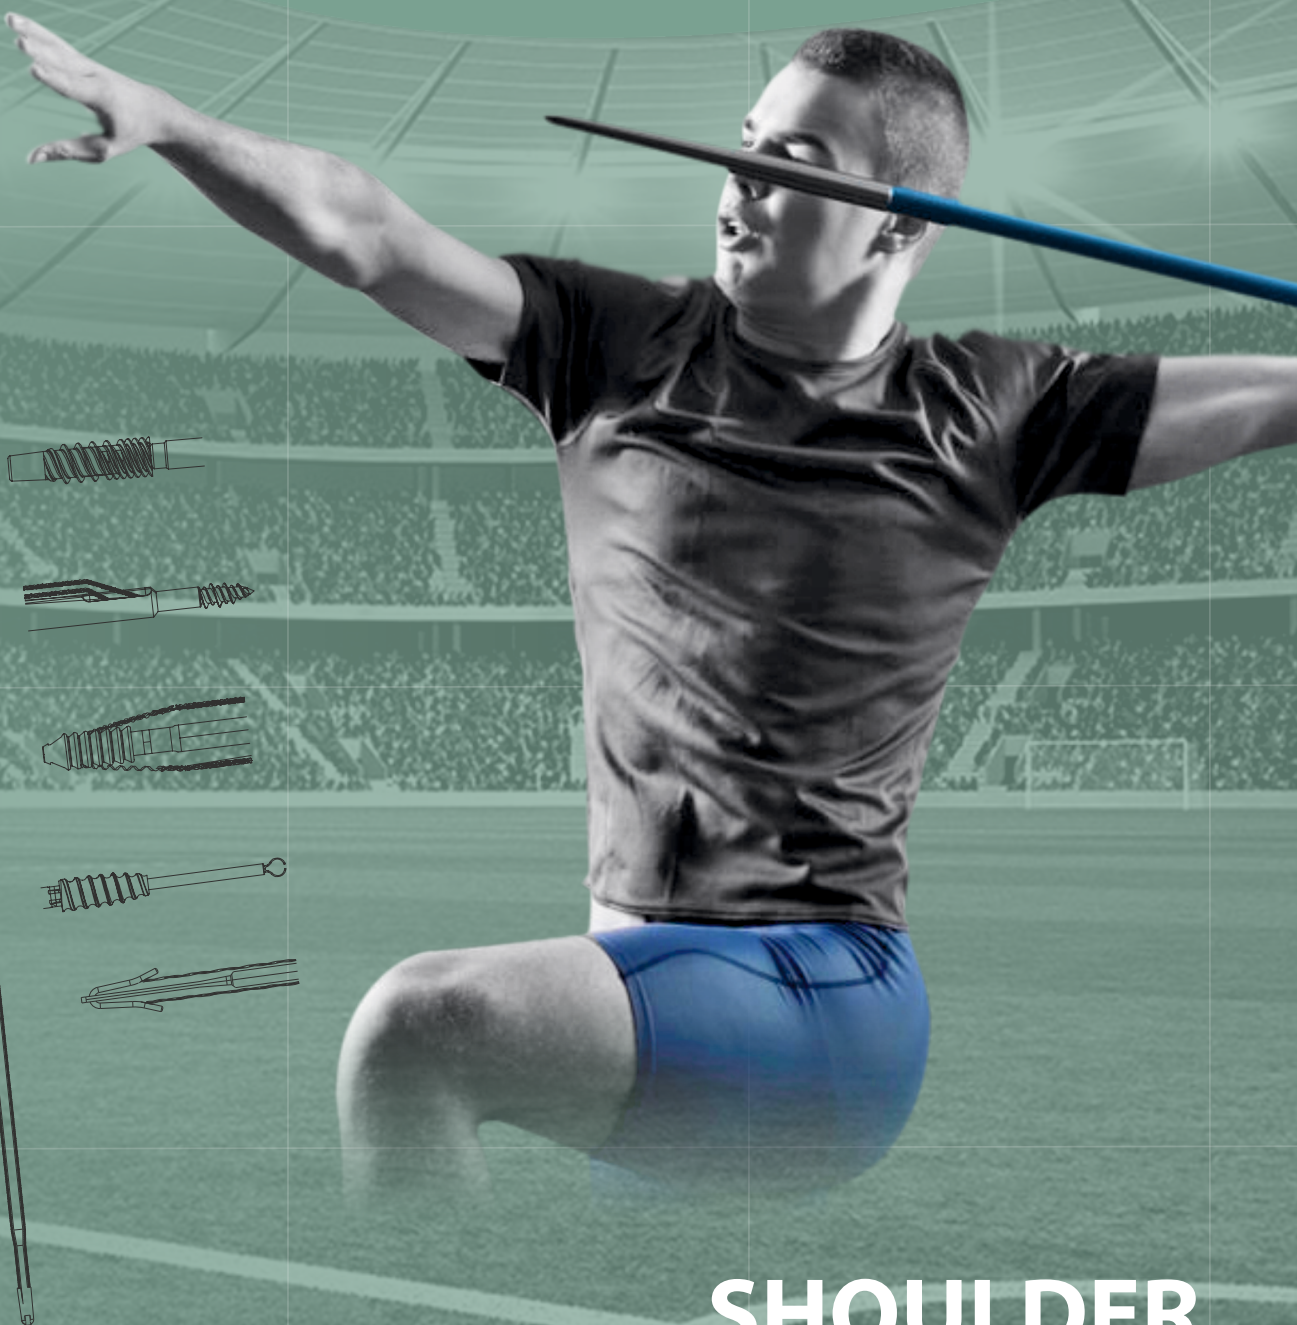





auxilock[®] 
SHOULDER Arthroscopy System

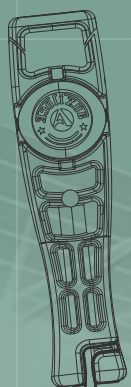

SHOULDER
Arthroscopy System

AUXILOCK[®] AUXPIK SUTURE-BASED ANCHOR

Rotator Cuff Repair

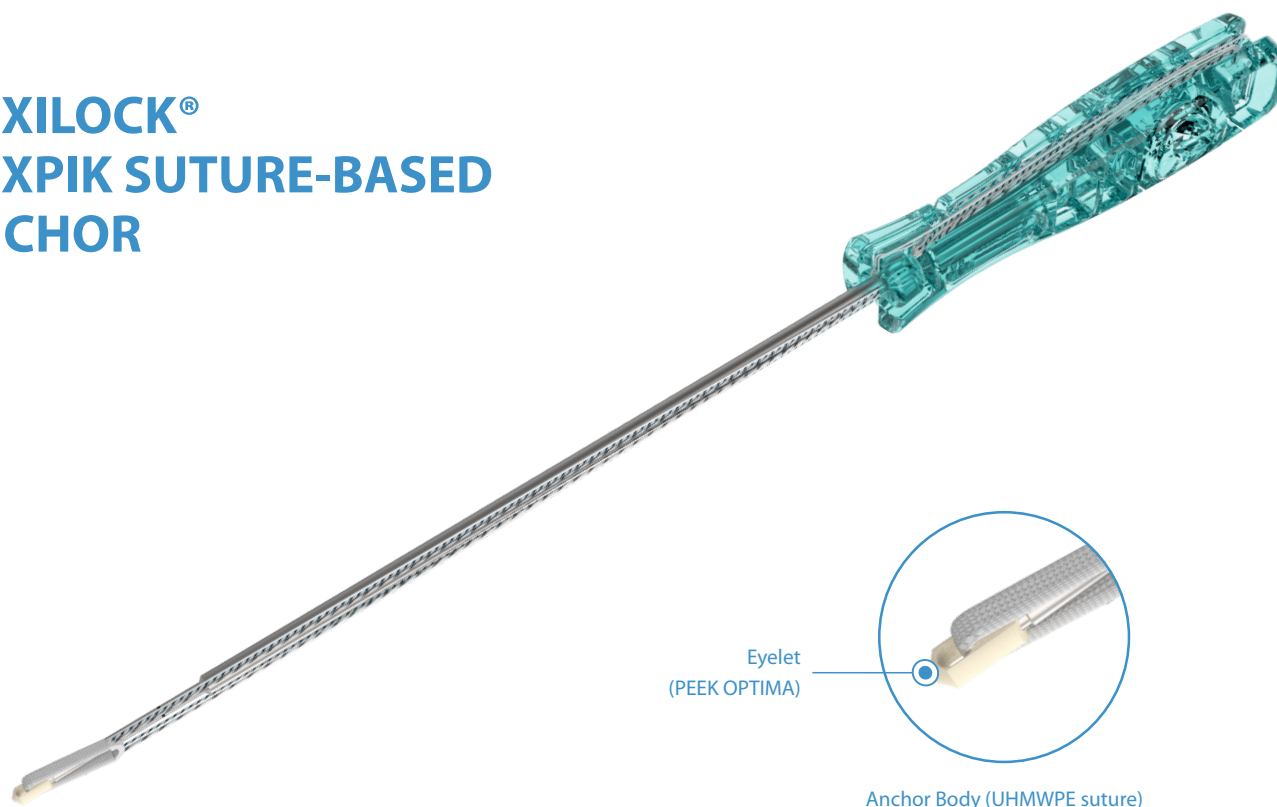

Eyelet
(PEEK OPTIMA)

Anchor Body (UHMWPE suture)

AUXILOCK[®] AuxPik suture-based anchor is made with UHMWPE suture anchor body and PEEK OPTIMA eyelet tip. The anchor is designed to deliver efficiency and promote ease of use. The AuxPik suture-based anchor is available in 3.2mm diameter with various combination of BioBraid and suture tapes. It can be used for rotator cuff repair surgeries. The AUXILOCK[®] AuxPik suture-based anchor provides a small footprint and also asserts subcortical fixation for anchor insertion. The drill guide and anchor driver combination is well designed to improve the performance and reliability.

Ordering Information


Code	Product Description	Suture/Tape Colour
6-001-03	AUXILOCK [®] 3.2mm AuxPik Suture-Based Anchor With Two #2 BioBraid: White/Blue & White/Black	
6-001-09	AUXILOCK [®] 3.2mm AuxPik Suture-Based Anchor With One #2 BioBraid and One 1.4mm Suture Tape: White/Black & White/Blue	

Recommended Instrumentation

Code	Product Description	Compatible Implants
7-013-01	8 Point Slotted Drill Guide, Length 190mm	6-001-03, 6-001-09
7-013-13	Ø3.2mm X 200mm Drill Bit	6-001-03, 6-001-09
7-013-23	Ø3.2mm Awl	6-001-03, 6-001-09
7-013-02	8 Point Drill Guide, Length 100mm	6-001-03, 6-001-09

STERILE EO

AUXILOCK[®] AUXSUTURE ANCHOR

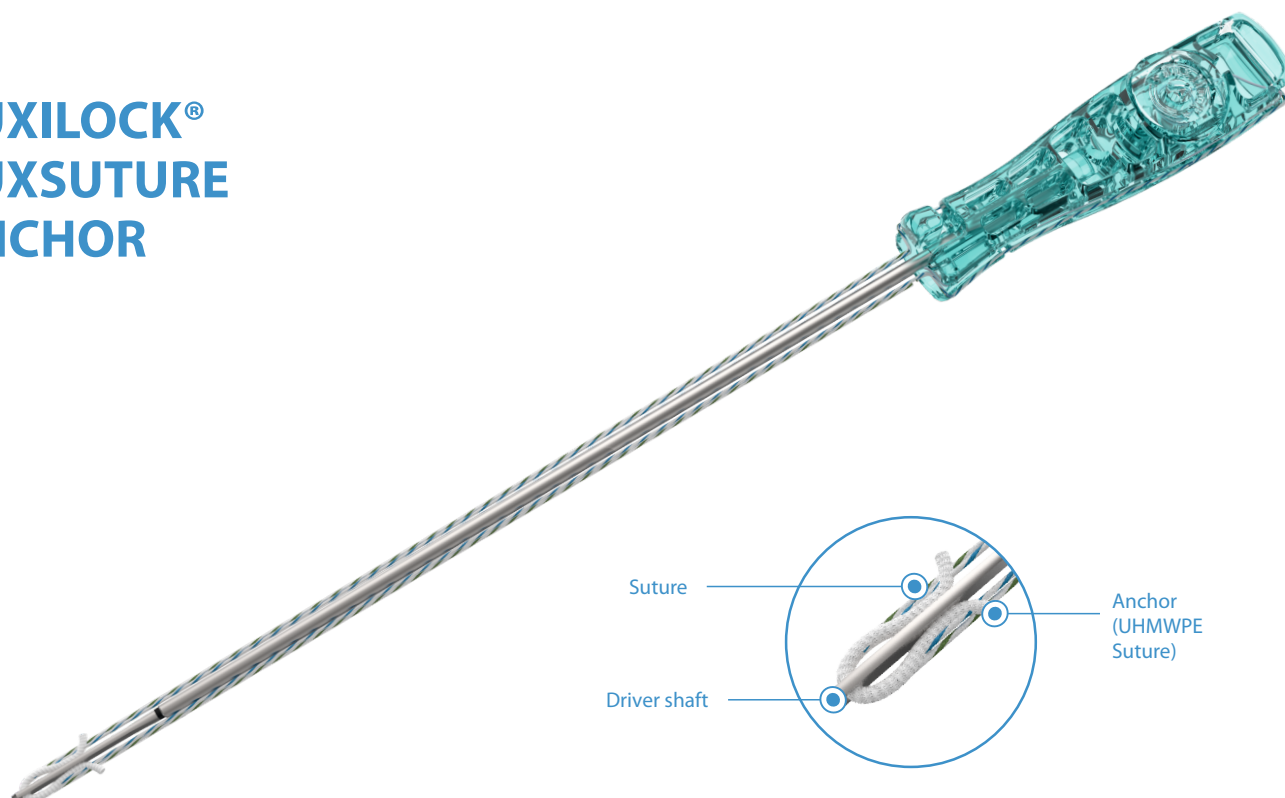

Rotator Cuff Repair

AUXILOCK[®] AuxSuture Anchor provides numerous advantages over traditional anchors. The strong fixation, less bone removal and a push in technique provide higher efficiency in rotator cuff repair procedures. AuxSuture anchor is available in diameter of 2.9mm. It requires a pilot hole for its insertion. The specially designed 2.9mm Awl for AuxSuture Anchor provides an accurate hole placement for the anchor. The small 2.9mm footprint of AuxSuture anchor provides placement and fixation advantages when bone real estate is limited, especially during revision surgeries. AuxSuture Anchor is available in double and triple loaded options with various combination of BioBraid and suture tapes.

Ordering Information

Code	Product Description	Suture/Tape Colour	Needle
6-036-01	AUXILOCK [®] 2.9mm AuxSuture Anchor With Two #2 BioBraid: White/Blue & White/Green		
6-036-02	AUXILOCK [®] 2.9mm AuxSuture Anchor With Two #2 BioBraid: White/Blue & White/Green, With Needle: MO-6		
6-036-03	AUXILOCK [®] 2.9mm AuxSuture Anchor With Three #2 BioBraid: White, White/Blue & White/Green		
6-036-04	AUXILOCK [®] 2.9mm AuxSuture Anchor With One #2 BioBraid and One 1.4mm Suture Tape: White/Black & White/Blue		
6-036-05	AUXILOCK [®] 2.9mm AuxSuture Anchor With Two 1.4mm Suture Tape: White/Black & White/Blue		


Recommended Instrumentation

Code	Product Description	Compatible Implants
7-013-22	Ø2.9mm Awl	6-036-01, 6-036-02, 6-036-03, 6-036-04, 6-036-05

STERILE EO

AUXILOCK[®] PEEK CF SCREW-IN SUTURE ANCHOR

Rotator Cuff Repair

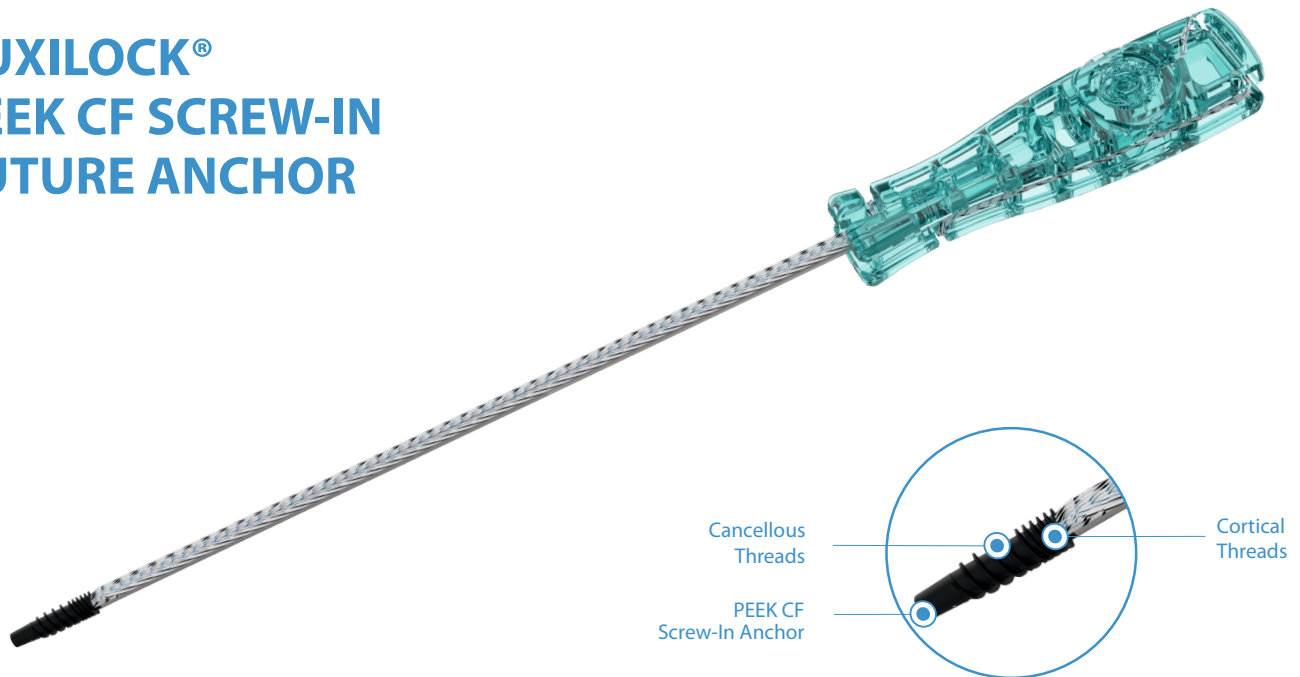







AUXILOCK[®] PEEK CF Screw-In Suture anchor is a fully threaded suture anchor featuring dual threads to maximize cortical and cancellous fixation. It is available in diameter of 4.5, 5.5 and 6.5mm with double and triple loaded options. It has a flat tip to protect the sutures and to facilitate the insertion. The anchor is particularly suitable for repairing rotator cuff and associated pathologies.

Ordering Information

Code	Product Description	Suture/Tape Colour
6-046-01	AUXILOCK [®] 4.5mm PEEK CF Screw-In Suture Anchor With Three #2 BioBraid: White, White/Blue & White/Black	
6-046-02	AUXILOCK [®] 4.5mm PEEK CF Screw-In Suture Anchor With Two #2 BioBraid: White/Blue & White/Black	
6-046-03	AUXILOCK [®] 5.5mm PEEK CF Screw-In Suture Anchor With Three #2 BioBraid: White, White/Blue & White/Black	
6-046-04	AUXILOCK [®] 5.5mm PEEK CF Screw-In Suture Anchor With Two #2 BioBraid: White/Blue & White/Black	
6-046-05	AUXILOCK [®] 6.5mm PEEK CF Screw-In Suture Anchor With Two #2 BioBraid: White/Blue & White/Black	
6-046-06	AUXILOCK [®] 4.5mm PEEK CF Screw-In Suture Anchor With One #2 BioBraid and One 1.4mm Suture Tape: White/Black & White/Blue	
6-046-07	AUXILOCK [®] 5.5mm PEEK CF Screw-In Suture Anchor With One #2 BioBraid and One 1.4mm Suture Tape: White/Black & White/Blue	
6-046-08	AUXILOCK [®] 6.5mm PEEK CF Screw-In Suture Anchor With One #2 BioBraid and One 1.4mm Suture Tape: White/Black & White/Blue	
6-046-09	AUXILOCK [®] 4.5mm PEEK CF Screw-In Suture Anchor With Two 1.4mm Suture Tape: White/Blue & White/Black	
6-046-10	AUXILOCK [®] 5.5mm PEEK CF Screw-In Suture Anchor With Two 1.4mm Suture Tape: White/Blue & White/Black	
6-046-11	AUXILOCK [®] 6.5mm PEEK CF Screw-In Suture Anchor With Two 1.4mm Suture Tape: White/Blue & White/Black	

Ordering Information

Code	Product Description	Suture/Tape Colour	Needle
6-016-21	AUXILOCK [®] 4.5mm PEEK CF Screw-In Suture Anchor With Two #2 BioBraid: White & White/Blue, With Needles: MO-6		
6-016-22	AUXILOCK [®] 5.5mm PEEK CF Screw-In Suture Anchor With Two #2 BioBraid: White & White/Blue, With Needles: MO-6		
6-016-23	AUXILOCK [®] 6.5mm PEEK CF Screw-In Suture Anchor With Two #2 BioBraid: White & White/Blue, With Needles: MO-6		


Recommended Instrumentation

Code	Product Description	Bone Density	Compatible Implants
7-013-25	Awl For 4.5/5.5mm PEEK Screw-In Anchor	Soft Bone	6-046-01, 6-046-02, 6-046-03, 6-046-04, 6-046-06, 6-046-07, 6-046-09, 6-046-10, 6-046-21, 6-046-22
7-013-26	Awl For 6.5mm PEEK Screw-In Anchor		6-046-05, 6-046-08, 6-046-11, 6-046-23
7-013-27	Awl/ Tap For 4.5/5.5mm PEEK Screw-In Anchor	Normal Bone	6-046-01, 6-046-02, 6-046-03, 6-046-04, 6-046-06, 6-046-07, 6-046-09, 6-046-10, 6-046-21, 6-046-22
7-013-28	Awl/ Tap For 6.5mm PEEK Screw-In Anchor		6-046-05, 6-046-08, 6-046-11, 6-046-23
7-013-29	Tap For 4.5/5.5mm PEEK Screw-In Anchor	Hard Bone	6-046-01, 6-046-02, 6-046-03, 6-046-04, 6-046-06, 6-046-07, 6-046-09, 6-046-10, 6-046-21, 6-046-22
7-013-30	Tap For 6.5mm PEEK Screw-In Anchor		6-046-05, 6-046-08, 6-046-11, 6-046-23

STERILE EO

AUXILOCK[®] PEEK OPTIMA SCREW-IN SUTURE ANCHOR

Rotator Cuff Repair

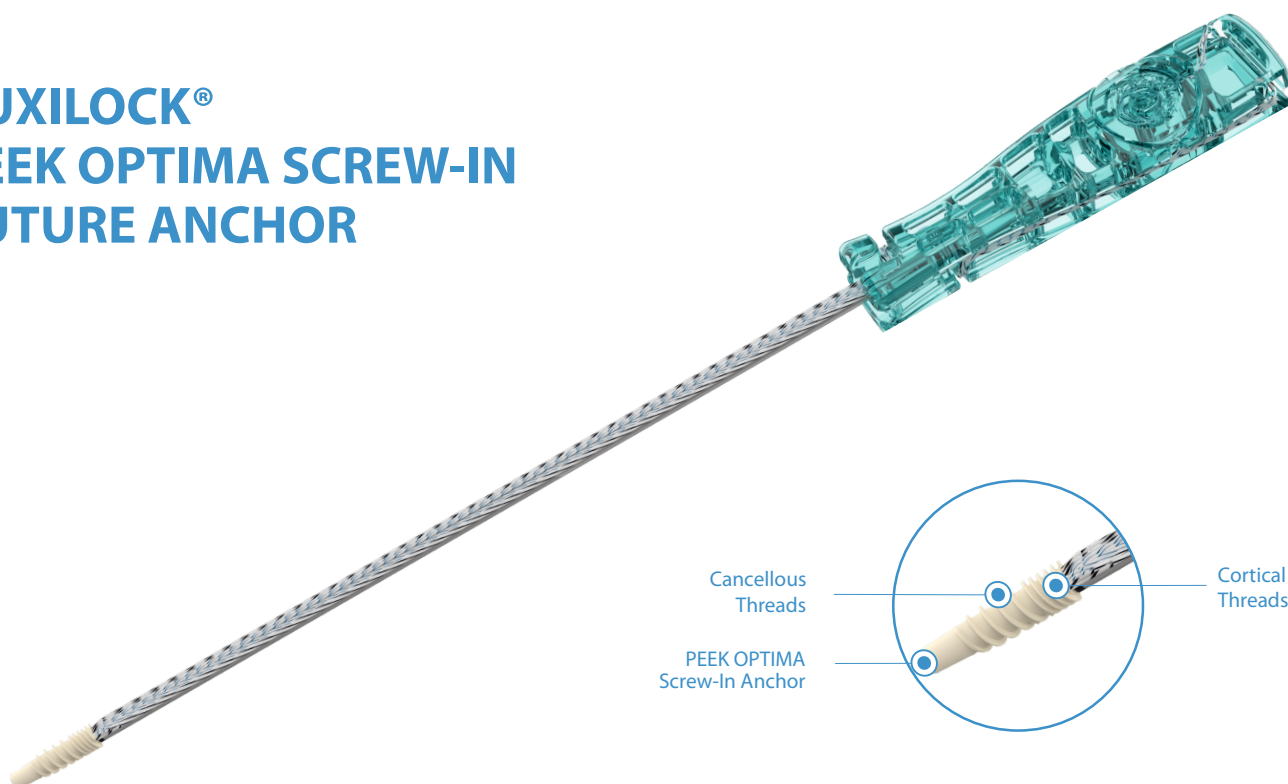







AUXILOCK[®] PEEK OPTIMA Screw-In Suture anchor is a fully threaded suture anchor featuring dual threads to maximize cortical and cancellous fixation. It is available in diameter of 4.5, 5.5 and 6.5mm with double and triple loaded options. It has a flat tip to protect the sutures and to facilitate the insertion. The anchor is particularly suitable for repairing rotator cuff and associated pathologies. The anchors are also available with needles which are ideal for mini-open rotator cuff repair procedures.

Ordering Information

Code	Product Description	Suture/Tape Colour
6-016-05	AUXILOCK [®] 4.5mm PEEK OPTIMA Screw-In Suture Anchor With Two #2 BioBraid: White/Blue & White/Black	
6-016-07	AUXILOCK [®] 5.5mm PEEK OPTIMA Screw-In Suture Anchor With Two #2 BioBraid: White/Blue & White/Black	
6-016-08	AUXILOCK [®] 6.5mm PEEK OPTIMA Screw-In Suture Anchor With Two #2 BioBraid: White/Blue & White/Black	
6-016-13	AUXILOCK [®] 4.5mm PEEK OPTIMA Screw-In Suture Anchor With Three #2 BioBraid: White, White/Blue & White/Black	
6-016-14	AUXILOCK [®] 5.5mm PEEK OPTIMA Screw-In Suture Anchor With Three #2 BioBraid: White, White/Blue & White/Black	
6-016-15	AUXILOCK [®] 4.5mm PEEK OPTIMA Screw-In Suture Anchor With One #2 BioBraid and One 1.4mm Suture Tape: White/Blue & White/Black	
6-016-16	AUXILOCK [®] 5.5mm PEEK OPTIMA Screw-In Suture Anchor With One #2 BioBraid and One 1.4mm Suture Tape: White/Blue & White/Black	
6-016-17	AUXILOCK [®] 6.5mm PEEK OPTIMA Screw-In Suture Anchor With One #2 BioBraid and One 1.4mm Suture Tape: White/Blue & White/Black	
6-016-18	AUXILOCK [®] 4.5mm PEEK OPTIMA Screw-In Suture Anchor With Two 1.4mm Suture Tape: White/Blue & White/Black	
6-016-19	AUXILOCK [®] 5.5mm PEEK OPTIMA Screw-In Suture Anchor With Two 1.4mm Suture Tape: White/Blue & White/Black	
6-016-20	AUXILOCK [®] 6.5mm PEEK OPTIMA Screw-In Suture Anchor With Two 1.4mm Suture Tape: White/Blue & White/Black	

Ordering Information

Code	Product Description	Suture/Tape Colour	Needle
6-016-01	AUXILOCK [®] 4.5mm PEEK OPTIMA Screw-In Suture Anchor With Two #2 BioBraid: White & White/Blue, With Needles: MO-6		
6-016-03	AUXILOCK [®] 5.5mm PEEK OPTIMA Screw-In Suture Anchor With Two #2 BioBraid: White & White/Blue, With Needles: MO-6		
6-016-04	AUXILOCK [®] 6.5mm PEEK OPTIMA Screw-In Suture Anchor With Two #2 BioBraid: White & White/Blue, With Needles: MO-6		


Recommended Instrumentation

Code	Product Description	Bone Density	Compatible Implants
7-013-25	Awl For 4.5/5.5mm PEEK Screw-In Anchor	Soft Bone	6-016-05, 6-016-07, 6-016-13, 6-016-14, 6-016-15, 6-016-16, 6-016-18, 6-016-19, 6-016-01, 6-016-03
7-013-26	Awl For 6.5mm PEEK Screw-In Anchor		6-016-08, 6-016-17, 6-016-20, 6-016-04
7-013-27	Awl/ Tap For 4.5/5.5mm PEEK Screw-In Anchor	Normal Bone	6-016-05, 6-016-07, 6-016-13, 6-016-14, 6-016-15, 6-016-16, 6-016-18, 6-016-19, 6-016-01, 6-016-03
7-013-28	Awl/ Tap For 6.5mm PEEK Screw-In Anchor		6-016-08, 6-016-17, 6-016-20, 6-016-04
7-013-29	Tap For 4.5/5.5mm PEEK Screw-In Anchor	Hard Bone	6-016-05, 6-016-07, 6-016-13, 6-016-14, 6-016-15, 6-016-16, 6-016-18, 6-016-19, 6-016-01, 6-016-03
7-013-30	Tap For 6.5mm PEEK Screw-In Anchor		6-016-08, 6-016-17, 6-016-20, 6-016-04

STERILE EO

AUXILOCK[®] TITANIUM SCREW-IN SUTURE ANCHOR

Rotator Cuff Repair

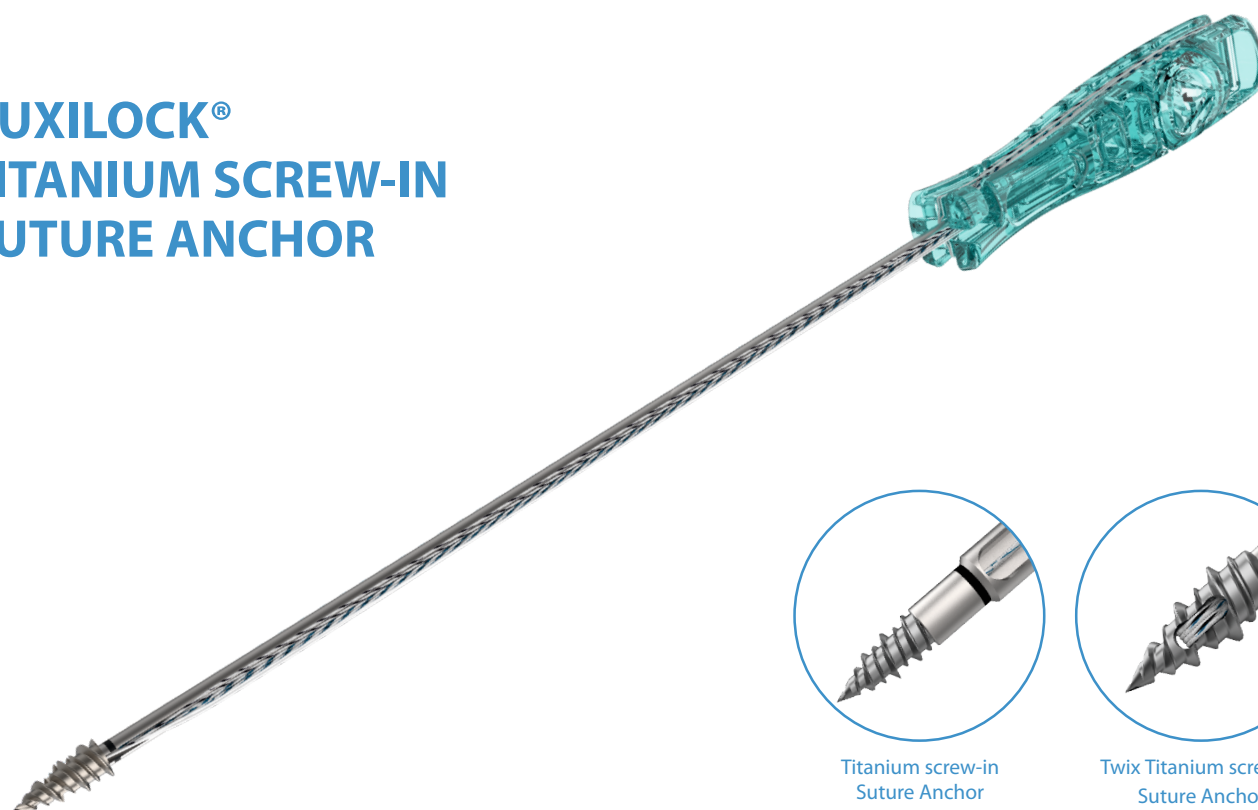

Titanium screw-in
Suture Anchor

Twix Titanium screw-in
Suture Anchor


The self-tapping AUXILOCK[®] Titanium screw-in suture anchor is mostly used as a medial row anchor in rotator cuff repair surgery. It is recommended for use in small and large-joint repairs without the need for tapping or drilling. AUXILOCK[®] Titanium screw-in anchors are available in diameter of 5.0 and 6.5mm with double and triple loaded options. The anchor design incorporates a cancellous thread with a very small core diameter to maximize pull-out strength in cancellous or osteoporotic bone. The anchor is designed for ultimate mechanical properties (pull-out strength, tensile strength, etc.) and ease-of-use. The anchors are also available with needles which are ideal for mini-open rotator cuff repair procedures.

Ordering Information

Code	Product Description	Suture/Tape Colour	Needle
6-004-02	AUXILOCK [®] 5.0mm Titanium Screw-In Suture Anchor With Two #2 BioBraid: White/Blue & White/Black		
6-004-13	AUXILOCK [®] 5.0mm Titanium Screw-In Suture Anchor With Three #2 BioBraid: White, White/Blue & White/Black		
6-004-05	AUXILOCK [®] 5.0mm Titanium Screw-In Suture Anchor With Two #2 BioBraid: White & White/Blue, With Needles: MO-6		
6-004-04	AUXILOCK [®] 6.5mm Titanium Screw-In Suture Anchor With Two #2 BioBraid: White/Blue & White/Black		
6-004-06	AUXILOCK [®] 6.5mm Titanium Screw-In Suture Anchor With Two #2 BioBraid: White & White/Blue, With Needles: MO-6		
6-045-01	AUXILOCK [®] 5.0mm Twix Titanium Screw-In Suture Anchor With Two #2 BioBraid: White & White/Blue, With Needles: MO-6		
6-045-02	AUXILOCK [®] 6.5mm Twix Titanium Screw-In Suture Anchor With Two #2 BioBraid: White & White/Blue, With Needles: MO-6		

STERILE EO

AUXILOCK[®] KNOTLESS PEEK CF PUSH-IN SUTURE ANCHOR

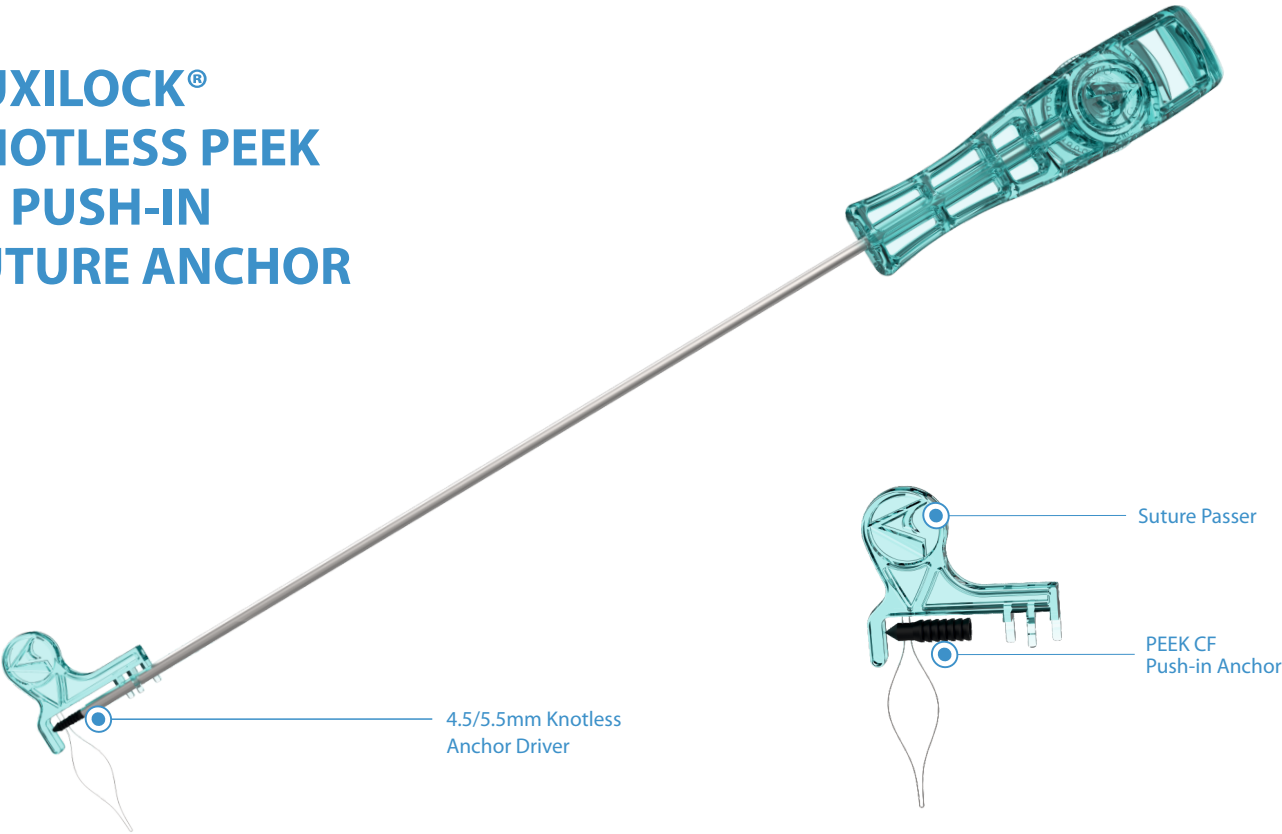

Rotator Cuff Repair

AUXILOCK[®] knotless push-in anchors provide a step-saving alternative to conventional knotted suture anchors. AUXILOCK[®] knotless push-in anchors are recommended for use in both large and small-joint soft tissue repairs. PEEK CF Push-In Suture Anchors consists of carbon fibre-reinforced PEEK OPTIMA and are available in a variety of diameters of 4.5mm and 5.5mm providing intraoperative flexibility. PEEK CF provides modulus of elasticity closely matching the cortical bone. It is non-absorbable, radiolucent, and MRI safe. The knotless technology of Push-in anchor also eliminates knot stacks associated with soft tissue irritation. The anchor is available with and without driver. The 4.5/5.5mm knotless anchor driver is provided separately in the instrument set. It is reusable driver that minimizes the cost of the surgery unlike the pre-loaded suture anchors.

Ordering Information


Code	Product Description
6-003-04	AUXILOCK [®] 4.5mm Knotless PEEK CF Push-In Suture Anchor With Suture Passer
6-003-05	AUXILOCK [®] 5.5mm Knotless PEEK CF Push-In Suture Anchor With Suture Passer
6-003-14	AUXILOCK [®] 4.5mm Knotless PEEK CF Push-In Suture Anchor With Driver, With Suture Passer
6-003-15	AUXILOCK [®] 5.5mm Knotless PEEK CF Push-In Suture Anchor With Driver, With Suture Passer

Recommended Instrumentation

Code	Product Description	Compatible Implants
7-013-23	Ø3.2mm Awl	6-003-04, 6-003-14
7-013-24	Ø4.1mm Awl	6-003-05, 6-003-15
7-013-32	4.5/5.5mm Knotless PEEK Anchor Driver	6-003-04, 6-003-05

STERILE EO

AUXILOCK[®] KNOTLESS PEEK OPTIMA PUSH-IN SUTURE ANCHOR

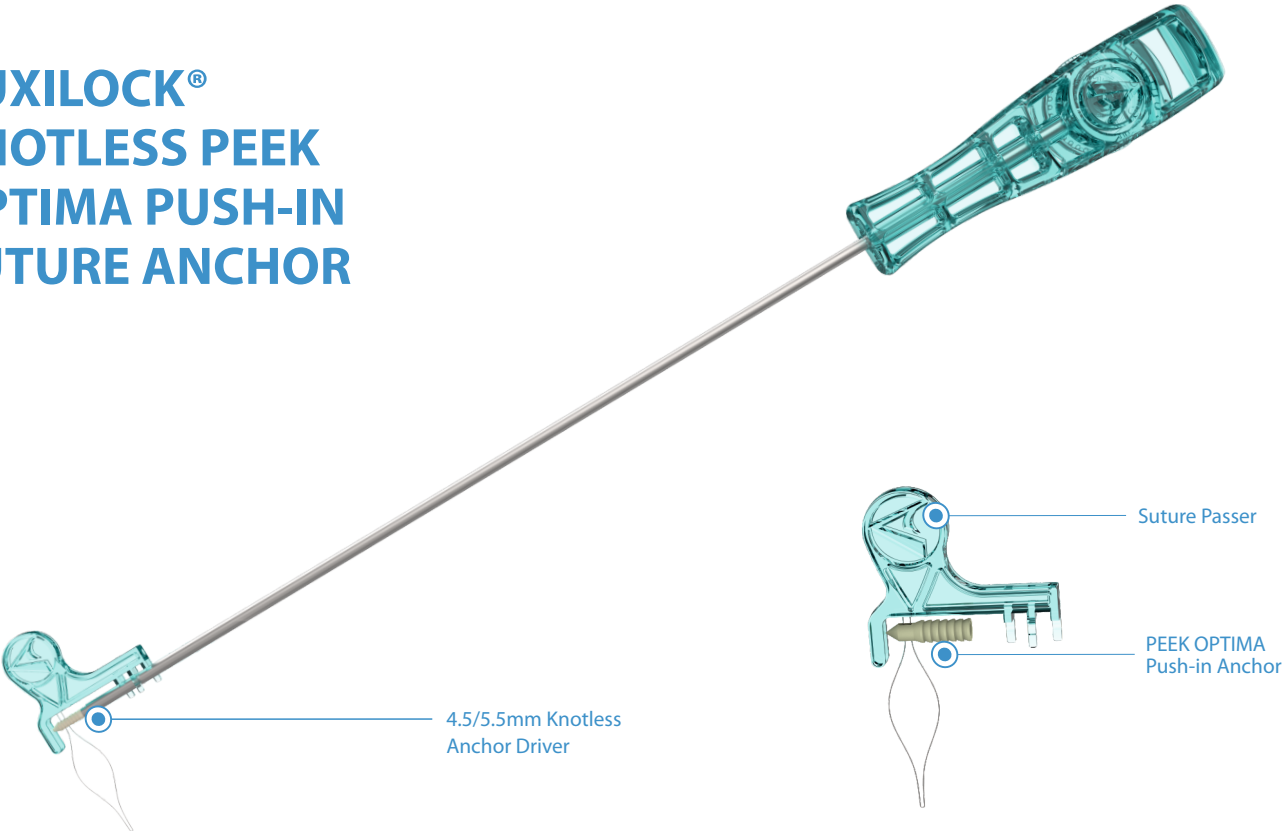

AUXILOCK[®] knotless push-in anchors provide a step-saving alternative to conventional knotted suture anchors. AUXILOCK[®] knotless push-in anchors are recommended for use in both large and small-joint soft tissue repairs. PEEK OPTIMA Push-In Suture Anchors consists of PEEK-OPTIMA (Poly-ether-ether-ketone) and are available in a variety of diameters of 4.5mm and 5.5mm providing intraoperative flexibility. The PEEK OPTIMA Push-In Suture Anchor is a non-absorbable PEEK suture anchor with a eyelet. Hence, providing superior abrasion resistance due to PEEK's low coefficient friction. It is biocompatible, radiolucent, and MRI safe. The knotless technology of Push-in anchor also eliminates knot stacks associated with soft tissue irritation. The anchor is available with and without driver. The 4.5/5.5mm knotless anchor driver is provided separately in the instrument set. It is reusable driver that minimizes the cost of the surgery unlike the pre-loaded suture anchors.

Ordering Information

Code	Product Description
6-031-04	AUXILOCK [®] 4.5mm Knotless PEEK OPTIMA Push-In Suture Anchor With Suture Passer
6-031-05	AUXILOCK [®] 5.5mm Knotless PEEK OPTIMA Push-In Suture Anchor With Suture Passer
6-031-07	AUXILOCK [®] 4.5mm Knotless PEEK OPTIMA Push In Suture Anchor With Driver, With Suture Passer
6-031-08	AUXILOCK [®] 5.5mm Knotless PEEK OPTIMA Push In Suture Anchor With Driver, With Suture Passer


Recommended Instrumentation

Code	Product Description	Compatible Implants
7-013-23	Ø3.2mm Awl	6-031-04, 6-031-07
7-013-24	Ø4.1mm Awl	6-031-05, 6-031-08
7-013-32	4.5/5.5mm Knotless PEEK Anchor Driver	6-031-04, 6-031-05

STERILE | EO

AUXILOCK[®] ROTADOR PEEK CF SCREW-IN ANCHOR

Rotator Cuff Repair

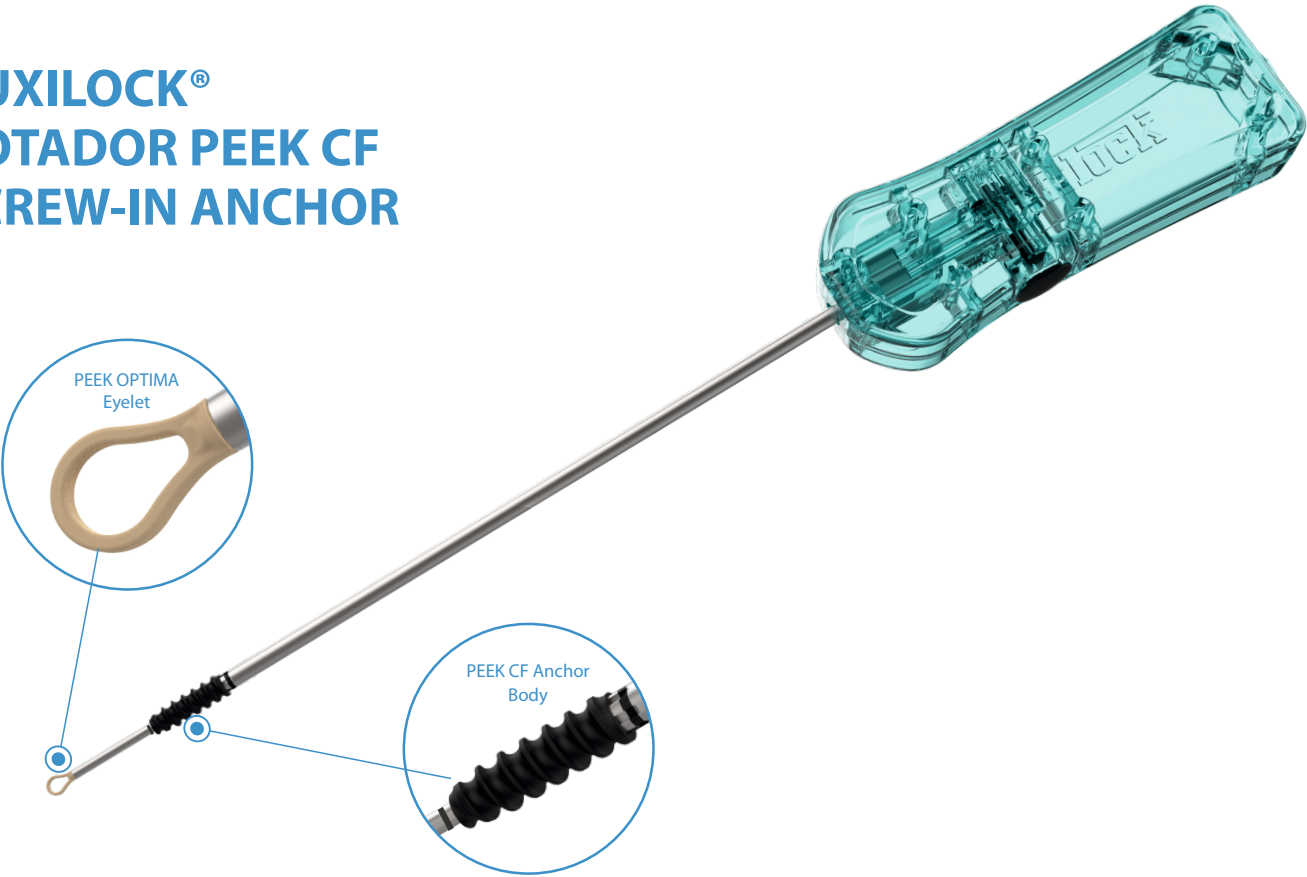

AUXILOCK[®] ROTADOR PEEK CF Screw-In Anchors are fully threaded knotless anchors available in 4.75, 5.5 and 6.25mm diameters with PEEK CF anchor body and PEEK OPTIMA eyelet. These anchors are designed to be used with sutures or tapes for rotator cuff repair using the 'bridge' techniques. Moreover, the 'knotless' technique consists of passing sutures or tapes of the medial row anchors through the tissue. They are finally inserted into the bone socket once they're loaded through the Rotador anchor eyelet. This technique eliminates possible complications caused by knots compared to other conventional anchors. The eyelet of the anchor accommodates up to 6 sutures and 2 tapes at a time.

Ordering Information

Code	Product Description
6-020-04	AUXILOCK [®] Rotador 4.75mm x 15mm PEEK CF Screw-In Anchor
6-020-05	AUXILOCK [®] Rotador 5.5mm x 15mm PEEK CF Screw-In Anchor
6-020-06	AUXILOCK [®] Rotador 6.25mm x 15mm PEEK CF Screw-In Anchor


Recommended Instrumentation

Code	Product Description	Compatible Implants
7-013-24	Ø4.1mm Awl	6-020-04, 6-020-05, 6-020-06

STERILE EO

AUXILOCK[®] ROTADOR PEEK OPTIMA SCREW-IN ANCHOR

Rotator Cuff Repair

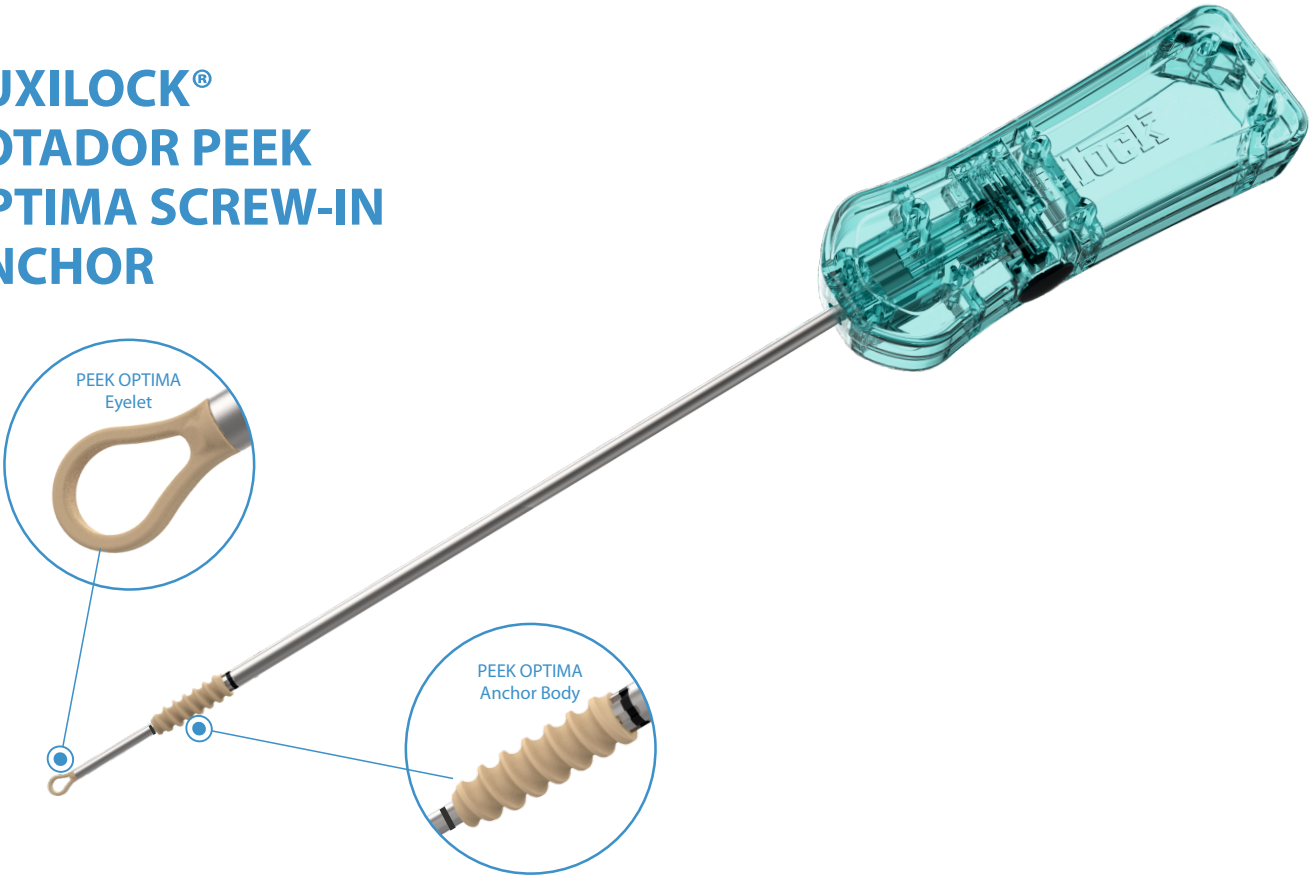

AUXILOCK[®] ROTADOR PEEK OPTIMA Screw-In Anchors are fully threaded knotless anchors available in 4.75, 5.5 and 6.25mm diameters with PEEK OPTIMA anchor body and eyelet. These anchors are designed to be used with sutures or tapes for rotator cuff repair using the 'bridge' technique. Moreover, the 'knotless' technique consists of passing sutures or tapes of the medial row anchors through the tissue. They are finally inserted into the bone socket once they're loaded through the Rotador anchor eyelet. This technique eliminates possible complications caused by knots compared to other conventional anchors. The eyelet of the anchor accommodates up to 6 sutures and 2 tapes at a time.

Ordering Information

Code	Product Description
6-020-01	AUXILOCK [®] Rotador 4.75mm x 15mm PEEK OPTIMA Screw-In Anchor
6-020-02	AUXILOCK [®] Rotador 5.5mm x 15mm PEEK OPTIMA Screw-In Anchor
6-020-03	AUXILOCK [®] Rotador 6.25mm x 15mm PEEK OPTIMA Screw-In Anchor

Recommended Instrumentation

Code	Product Description	Compatible Implants
7-013-24	Ø4.1mm Awl	6-020-01, 6-020-02, 6-020-03

STERILE EO

AUXILOCK[®] GYROLOCK PEEK OPTIMA KNOTLESS SCREW IN ANCHOR



Self-Punching
Eyelet

PEEK OPTIMA
Eyelet

PEEK OPTIMA
Anchor Body

Rotator Cuff Repair

GyroLock Knotless PEEK OPTIMA Screw-in Anchors consists of PEEK-OPTIMA (Poly-ether-ether-ketone) material. The GyroLock suture anchor comes with Dual start thread technology (fast inserting suture anchor) which allows anchor deployment in 3.5 rotation.

Vented and cannulated GyroLock anchors are designed for repair and reconstruction with soft-tissue graft. GyroLock anchor is available with multiple BioBraid suture and suture tape configurations.

The GyroLock is designed for multiple procedures in single or double row for lateral row applications. GyroLock suture anchor eyelet can accommodate up to four 1.4mm tapes or four #2 sutures.

Ordering Information

Code	Product Description	Silicon Color
6-052-02	AUXILOCK [®] GyroLock 4.75mm x 22.5mm Knotless PEEK OPTIMA Screw-In Anchor	Red
6-052-03	AUXILOCK [®] GyroLock 5.5mm x 22.5mm Knotless PEEK OPTIMA Screw-In Anchor	Blue
6-052-04	AUXILOCK [®] GyroLock SP 4.75mm x 24.5mm Knotless PEEK OPTIMA Screw-In Anchor, Self-Punching	Red
6-052-05	AUXILOCK [®] GyroLock SP 5.5mm x 24.5mm Knotless PEEK OPTIMA Screw-In Anchor, Self-Punching	Blue


Related Instrumentation

Code	Product Description
7-013-69	Awl/Tap for 4.75/5.5mm GyroLock Screw-In Anchor
7-013-70	Tap for 4.75/5.5mm GyroLock Screw-In Anchor

STERILE EO



AUXILOCK[®] AUXPIK SUTURE-BASED ANCHOR

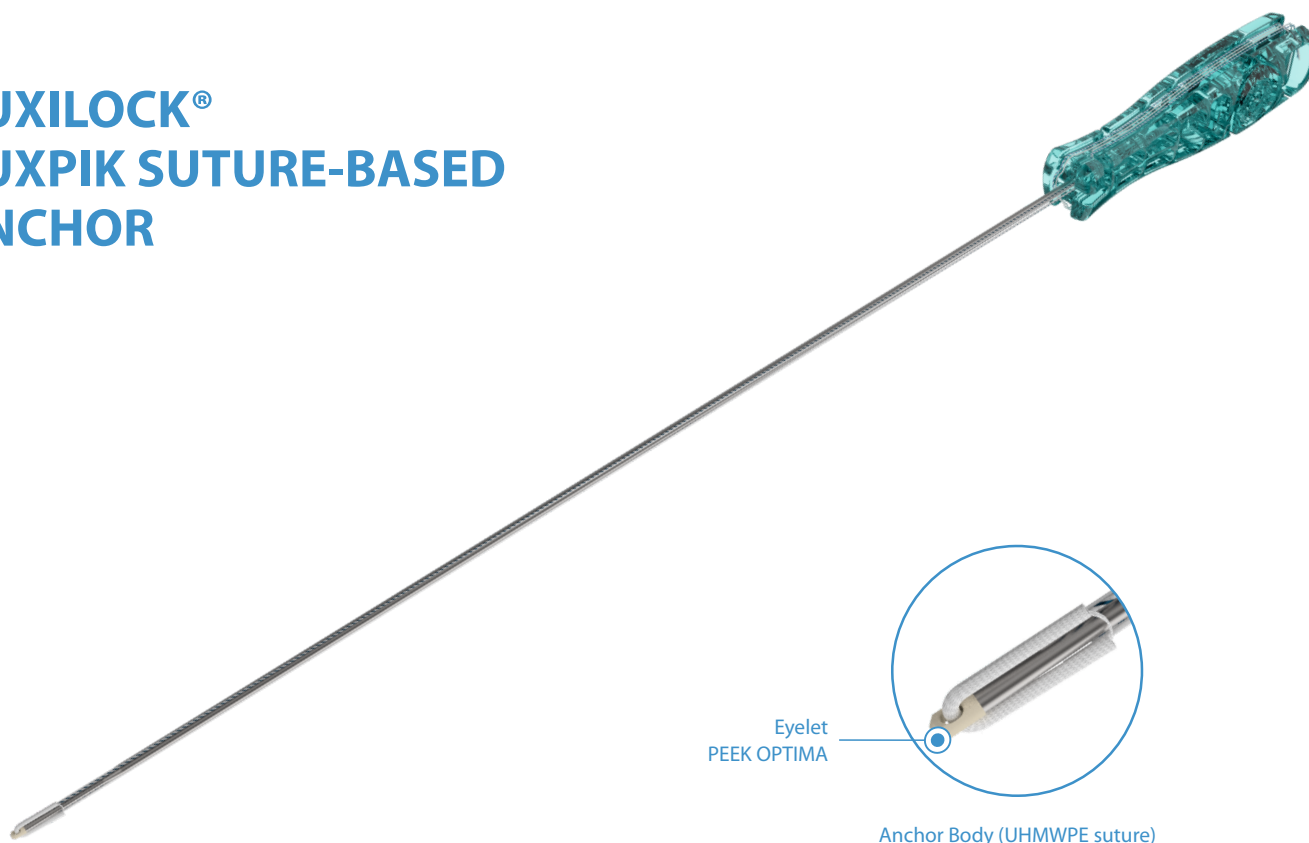Shoulder Instability Repair



AUXILOCK[®] AuxPik Suture-Based Anchor is made from UHMWPE suture anchor body with a PEEK OPTIMA eyelet tip. The AuxPik Suture-Based Anchor is designed for efficiency and ease of use. AuxPik Suture-Based Anchor is available in 1.8mm diameter with various combination of BioBraid and suture tapes. The anchor can be used for Bankart or SLAP repair surgeries. The anchor provides small foot print and subcortical fixation for anchor insertions. The drill guide and anchor driver combination are well designed to improve performance and reliability.

Ordering Information


Code	Product Description	Suture/Tape Colour
6-001-01	AUXILOCK [®] 1.8mm AuxPik Suture-Based Anchor With One #2 BioBraid: White/Blue	
6-001-08	AUXILOCK [®] 1.8mm AuxPik Suture-Based Anchor With One 1.4mm Suture Tape: White/Blue	

Recommended Instrumentation

Code	Product Description	Compatible Implants
7-013-03	V-Mouth Drill Guide	6-001-01, 6-001-08
7-013-04	8 Point Drill Guide	6-001-01, 6-001-08
7-013-06	Trocar Tip Obturator	6-001-01, 6-001-08
7-013-53	Ø1.8mm X 325mm Drill Bit	6-001-01, 6-001-08

STERILE EO

AUXILOCK[®] AUXSUTURE ANCHOR

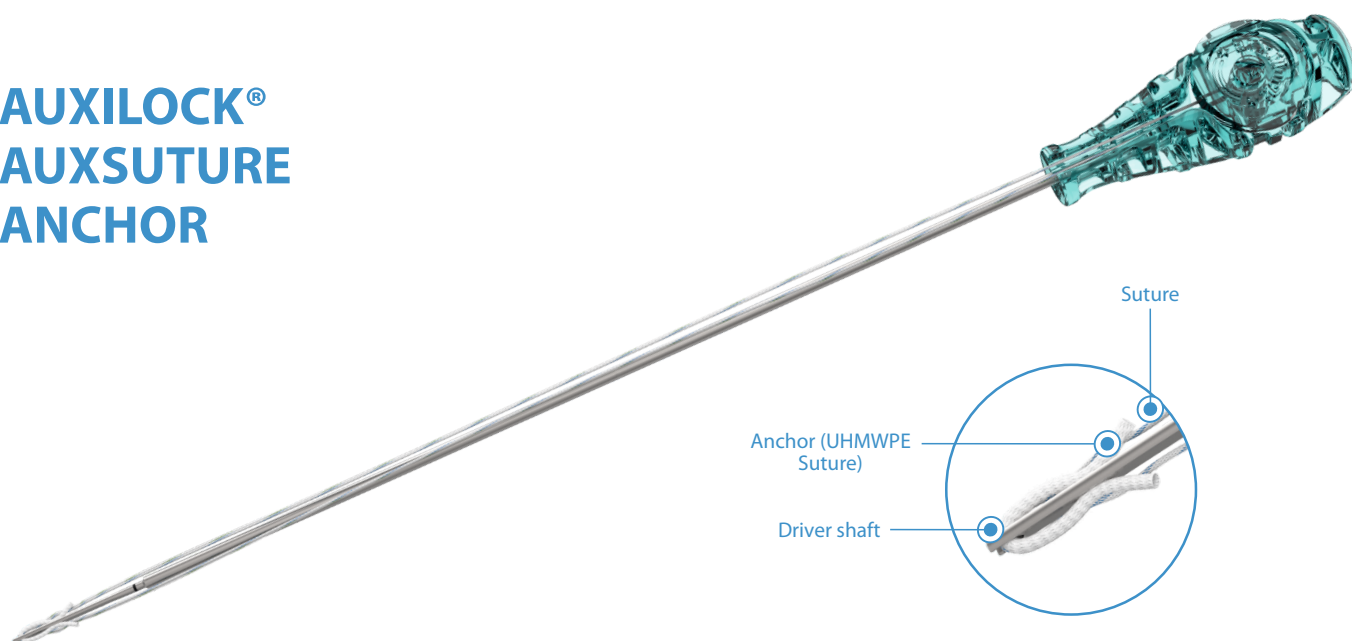

Shoulder Instability Repair

AUXILOCK[®] AuxSuture Anchor Provides numerous advantages over traditional anchors for shoulder instability repair procedures with its strong fixations, less bone removal and a push in techniques. AuxSuture anchor is available in diameter of 1.5mm and 1.8mm. It is available in single and double loaded options with various combination of BioBraid and suture tapes. The drill guide and 1.5mm drill bit are specially designed for AuxSuture Anchor while assuming an accurate hole placement for the anchor. The small 1.5mm footprint AuxSuture anchor provides placement and fixation advantages when bone real estate is limited, especially during revision surgeries. The anchor is also available with needles which are ideal for mini-open surgeries.

Ordering Information

Code	Product Description	Suture/Tape Colour	Needle
6-034-01	AUXILOCK [®] 1.5mm AuxSuture Anchor With One #2 BioBraid: White/Blue		
6-034-02	AUXILOCK [®] 1.5mm AuxSuture Anchor With One 1.4mm Suture Tape: White/Blue		
6-034-03	AUXILOCK [®] 1.5mm AuxSuture Anchor With One #2 BioBraid: White/Blue, With Needles: MO-6		
6-035-01	AUXILOCK [®] 1.8mm AuxSuture Anchor With Two #2 BioBraid: White/Blue & White/Green		
6-035-02	AUXILOCK [®] 1.8mm AuxSuture Anchor With One #2 BioBraid and One 1.4mm Suture Tape: White/Black & White/Blue		
6-035-03	AUXILOCK [®] 1.8mm AuxSuture Anchor With Two #2 BioBraid: White/Blue & White/Green, With Needles: MO-6		
6-035-04	AUXILOCK [®] 1.8mm AuxSuture Anchor With One #2 BioBraid and One 1.4mm Suture Tape: White/Black & White/Blue, With Needles: MO-6		


Recommended Instrumentation

Code	Product Description	Compatible Implants
7-013-03	V-Mouth Drill Guide	6-034-01, 6-034-02, 6-035-01, 6-035-02
7-013-04	8 Point Drill Guide	6-034-01, 6-034-02, 6-035-01, 6-035-02
7-013-05	V-Mouth Drill Guide - Curve	6-034-01, 6-034-02, 6-035-01, 6-035-02
7-013-06	Trocar Tip Obturator	6-034-01, 6-034-02, 6-035-01, 6-035-02
7-013-07	Trocar Tip Obturator - Curve	6-034-01, 6-034-02, 6-035-01, 6-035-02
7-013-20	Ø1.5mm X 300mm Drill Bit, Stainless Steel	6-034-01, 6-034-02, 6-034-03, 6-035-01, 6-035-02, 6-035-03, 6-035-04
7-013-21	Ø1.5mm X 300mm Drill Bit, Nitinol	6-034-01, 6-034-02, 6-035-01, 6-035-02
7-013-01	8 Point Slotted Drill Guide, Length 190mm	6-034-03, 6-035-03, 6-035-04
7-013-02	8 Point Drill Guide, Length 100mm	6-034-03, 6-035-03, 6-035-04

STERILE EO

AUXILOCK[®] PEEK CF PUSH-IN SUTURE ANCHOR

Shoulder Instability Repair

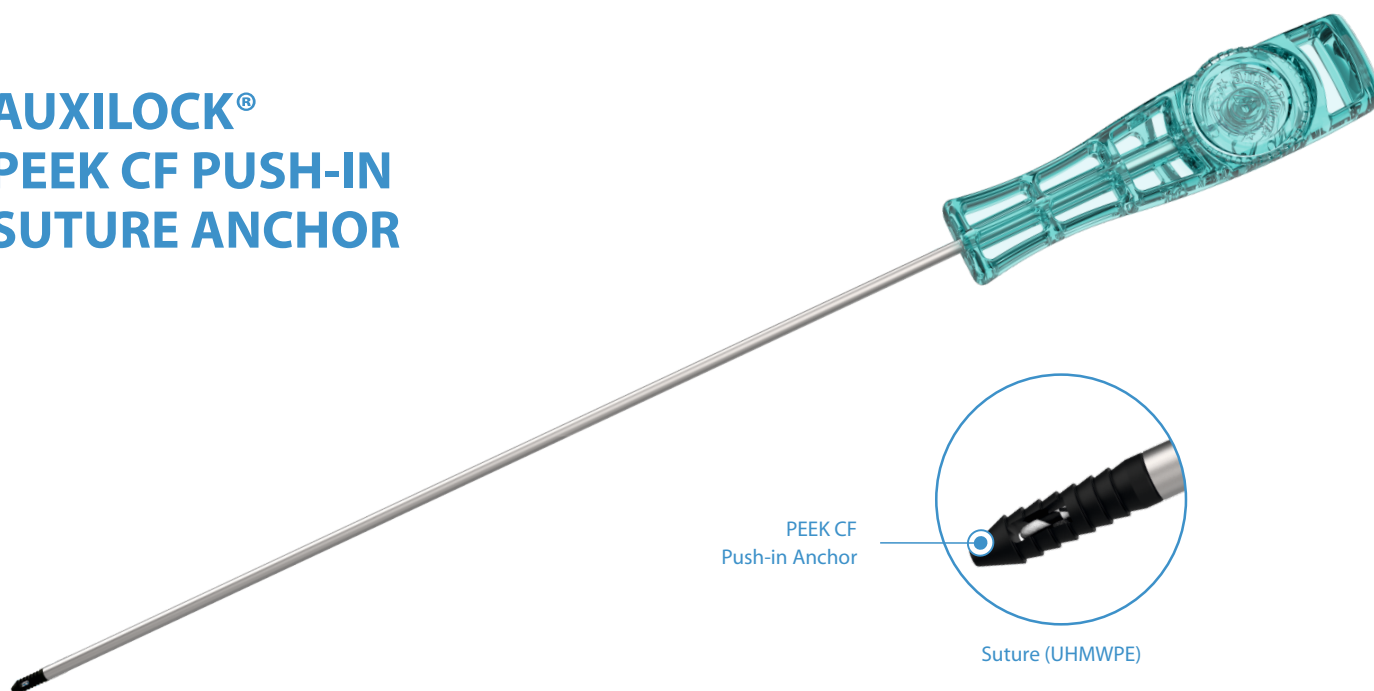

PEEK CF
Push-in Anchor

Suture (UHMWPE)

AUXILOCK[®] PEEK CF Push-In Suture Anchor is a Push-in/ Bang-on anchor available in diameter of 2.8 and 3.5mm. It is available in single and double loaded sutures with and without needle options. The PEEK CF Push-In Suture Anchors are made of carbon fiber-reinforced PEEK-OPTIMA. The PEEK CF provides modulus of elasticity closely matching the cortical bone. It is non-absorbable, radiolucent, and MRI safe. The drill guide and drill bit are provided in the instrument set for the accurate placement of the anchor which minimizes the anchor slippage or breakage during the surgery. Anchor insertion and delivery are made simple by drilling a hole through a drill guide and inserting the anchor through the same drill guide into the drilled hole. The anchor is also available with needles which are ideal for mini-open Bankart or SLAP repair procedures.

Ordering Information


Code	Product Description	Suture/Tape Colour	Needle
6-002-06	AUXILOCK [®] 2.8mm PEEK CF Push-In Suture Anchor With One #2 BioBraid: White/Blue		
6-002-07	AUXILOCK [®] 2.8mm PEEK CF Push-In Suture Anchor With One #2 BioBraid: White/Blue, With Needles: MO-6, Short Length		
6-002-01	AUXILOCK [®] 3.5mm PEEK CF Push-In Suture Anchor With Two #2 BioBraid: White/Blue & White/Black		
6-002-02	AUXILOCK [®] 3.5mm PEEK CF Push-In Suture Anchor With Two #2 BioBraid: White & White/Blue, With Needles: MO-6, Short Length		

Recommended Instrumentation

Code	Product Description	Compatible Implants
7-013-03	V-Mouth Drill Guide	6-002-06, 6-002-01
7-013-04	8 Point Drill Guide	6-002-06, 6-002-01
7-013-06	Trocar Tip Obturator	6-002-06, 6-002-01
7-013-17	Ø2.4mm X 300mm Drill Bit	6-002-06
7-013-18	Ø2.8mm X 300mm Drill Bit	6-002-01
7-013-01	8 Point Slotted Drill Guide, Length 190mm	6-002-07, 6-002-02
7-013-12	Ø2.4mm X 200mm Drill Bit	6-002-07
7-013-11	Ø2.8mm X 200mm Drill Bit	6-002-02
7-013-02	8 Point Drill Guide, Length 100mm	6-002-07, 6-002-02

STERILE EO

AUXILOCK[®] PEEK OPTIMA PUSH-IN SUTURE ANCHOR

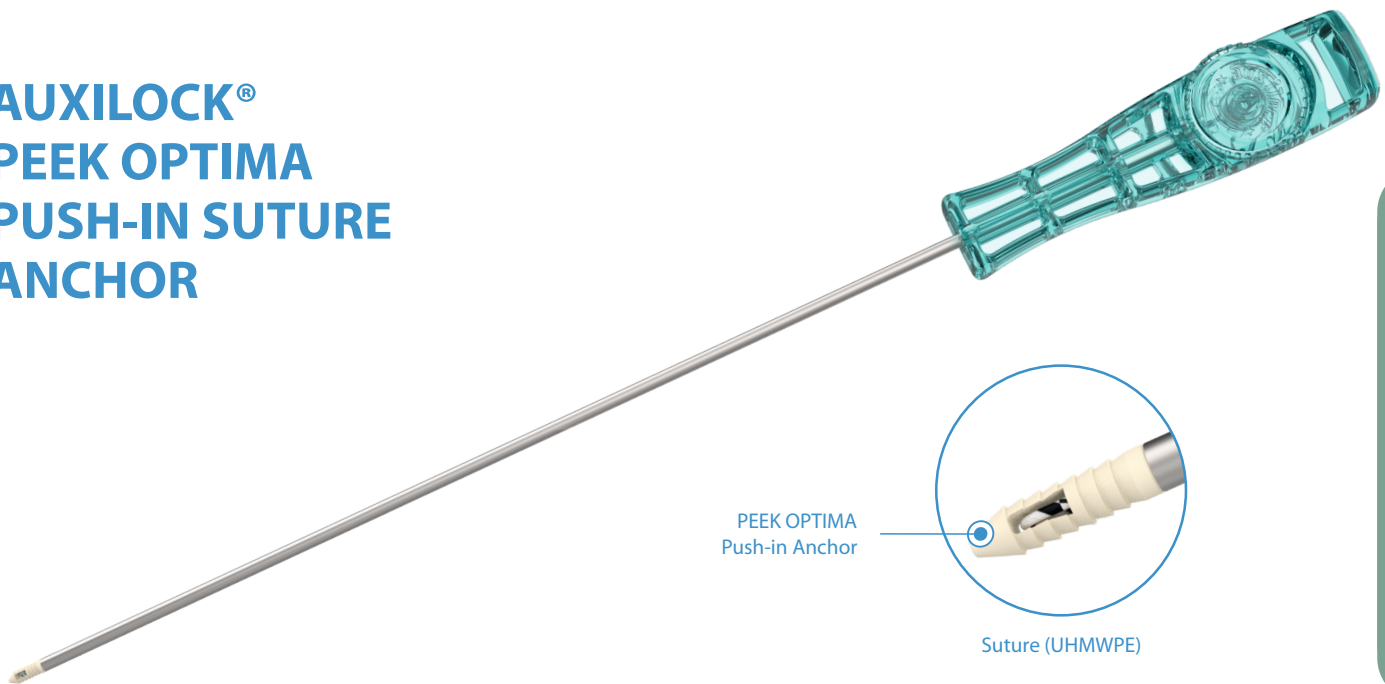

Shoulder Instability Repair

AUXILOCK[®] PEEK OPTIMA Push-In Suture Anchor is a Push-in/ Bang-on anchor available in diameter of 2.8 and 3.5mm. It is available in single and double loaded sutures with and without needle options. The PEEK OPTIMA Push-In Suture Anchors are made of PEEK-OPTIMA (Poly-ether-ether-ketone). The PEEK OPTIMA Push-In Suture Anchors are non-absorbable PEEK suture anchors with a material eyelet. It provides superior abrasion resistance due to PEEK's low coefficient friction. It is considered to be Biocompatible, radiolucent, and MRI safe. The drill guide and the drill bit are provided in the instrument set for an accurate placement of the anchor which minimizes the anchor slippage or breakage during the surgery. Anchor insertion and delivery are made simple by drilling a hole through a drill guide and inserting the anchor through the same drill guide into the drilled hole.

Ordering Information


Code	Product Description	Suture/Tape Colour	Needle
6-030-03	AUXILOCK [®] 2.8mm PEEK OPTIMA Push-In Suture Anchor With One #2 BioBraid: White/Black		
6-030-04	AUXILOCK [®] 2.8mm PEEK OPTIMA Push-In Suture Anchor With One #2 BioBraid: White/Black, With Needles: MO-6, Short Length		
6-030-01	AUXILOCK [®] 3.5mm PEEK OPTIMA Push-In Suture Anchor With Two #2 BioBraid: White/Blue & White/Black		
6-030-02	AUXILOCK [®] 3.5mm PEEK OPTIMA Push-In Suture Anchor With Two #2 BioBraid: White & White/Blue, With Needles: MO-6, Short Length		

Recommended Instrumentation

Code	Product Description	Compatible Implants
7-013-03	V-Mouth Drill Guide	6-030-03, 6-030-01
7-013-04	8 Point Drill Guide	6-030-03, 6-030-01
7-013-06	Trocar Tip Obturator	6-030-03, 6-030-01
7-013-17	Ø2.4mm X 300mm Drill Bit	6-030-03
7-013-18	Ø2.8mm X 300mm Drill Bit	6-030-01
7-013-01	8 Point Slotted Drill Guide, Length 190mm	6-030-04, 6-030-02
7-013-12	Ø2.4mm X 200mm Drill Bit	6-030-04, 6-030-02
7-013-11	Ø2.8mm X 200mm Drill Bit	6-030-04
7-013-02	8 Point Drill Guide, Length 100mm	6-030-02

STERILE EO

AUXILOCK[®] TITANIUM SCREW-IN SUTURE ANCHOR

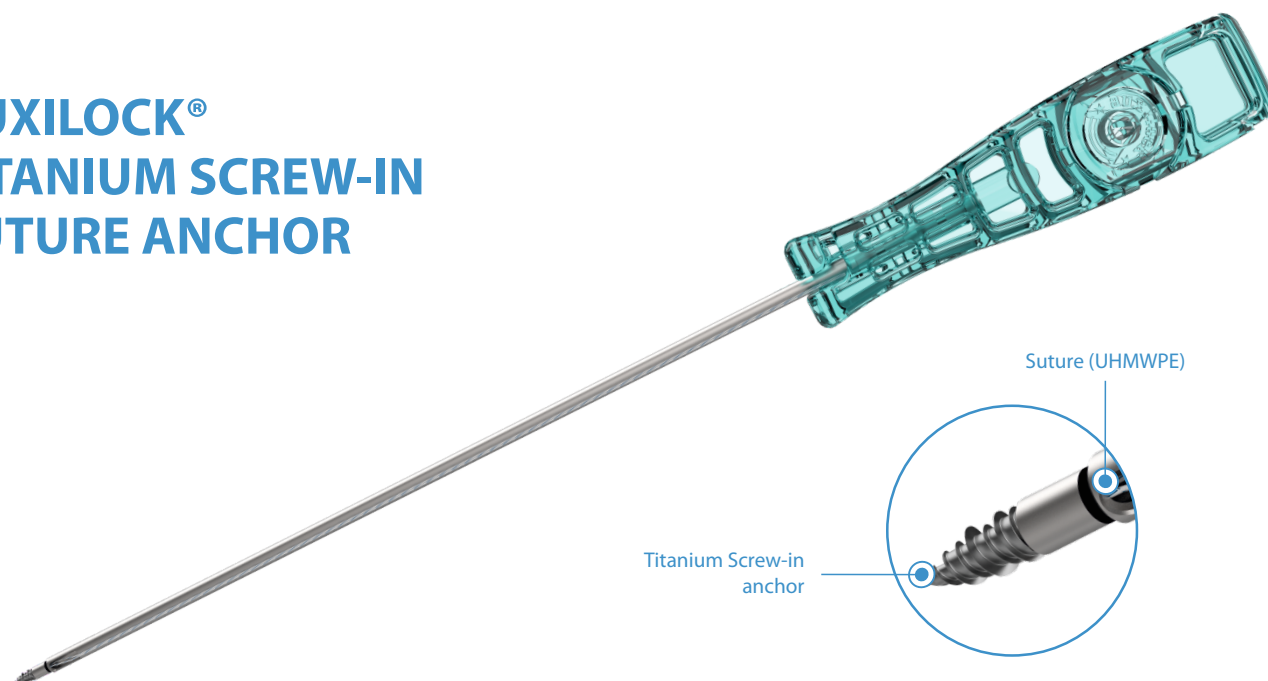

AUXILOCK[®] Titanium anchors are the screw-in anchors available in diameter of 2.8 and 3.5mm with single and double loaded options. It is a self-tapping suture anchor mostly used in Bankart or SLAP surgeries. The anchor design incorporates a cortical thread to maximise pull-out strength in a cortical or hard bone. The anchor is designed for delivering its ultimate mechanical properties (pull-out strength, tensile strength, etc.) and ease-of-use. The drill guide and drill bit are provided in the instrument set for the accurate placement of the anchor. It in turn minimizes the anchor slippage or breakage during the surgery. The anchors are also available with needles which are ideal for mini-open shoulder instability repair procedures.

Ordering Information

Code	Product Description	Suture/Tape Colour	Needle
6-005-01	AUXILOCK [®] 2.8mm Titanium Screw-In Suture Anchor With One #2 BioBraid: White/Blue		
6-005-05	AUXILOCK [®] 2.8mm Titanium Screw-In Suture Anchor With One #2 BioBraid: White/Blue, With Needles: MO-6		
6-005-02	AUXILOCK [®] 3.5mm Titanium Screw-In Suture Anchor With Two #2 BioBraid: White/Blue & White/Black		
6-005-06	AUXILOCK [®] 3.5mm Titanium Screw-In Suture Anchor With Two #2 BioBraid: White & White/Blue, With Needles: MO-6		
6-005-13	AUXILOCK [®] 3.5mm Titanium Screw-In Suture Anchor With One #2 BioBraid: White/Blue, With Needles: MO-6		
6-005-14	AUXILOCK [®] 3.5mm Titanium Screw-In Suture Anchor With One #2 BioBraid: White/Blue		


Recommended Instrumentation

Code	Product Description	Compatible Implants
7-013-03	V-Mouth Drill Guide	6-005-01, 6-005-02, 6-005-14
7-013-04	8 Point Drill Guide	6-005-01, 6-005-02, 6-005-14
7-013-06	Trocar Tip Obturator	6-005-01, 6-005-02, 6-005-14
7-013-16	Ø1.8mm X 300mm Drill Bit	6-005-01, 6-005-02, 6-005-14
7-013-02	8 Point Drill Guide, Length 100mm	6-005-05, 6-005-06, 6-005-13
7-013-10	Ø1.8mm X 200mm Drill Bit	6-005-05, 6-005-06, 6-005-13
7-013-01	8 Point Slotted Drill Guide, Length 190mm	6-005-05, 6-005-06, 6-005-13

STERILE EO

AUXILOCK[®]
KNOTLESS PEEK
CF PUSH-IN
SUTURE ANCHOR

Shoulder Instability Repair

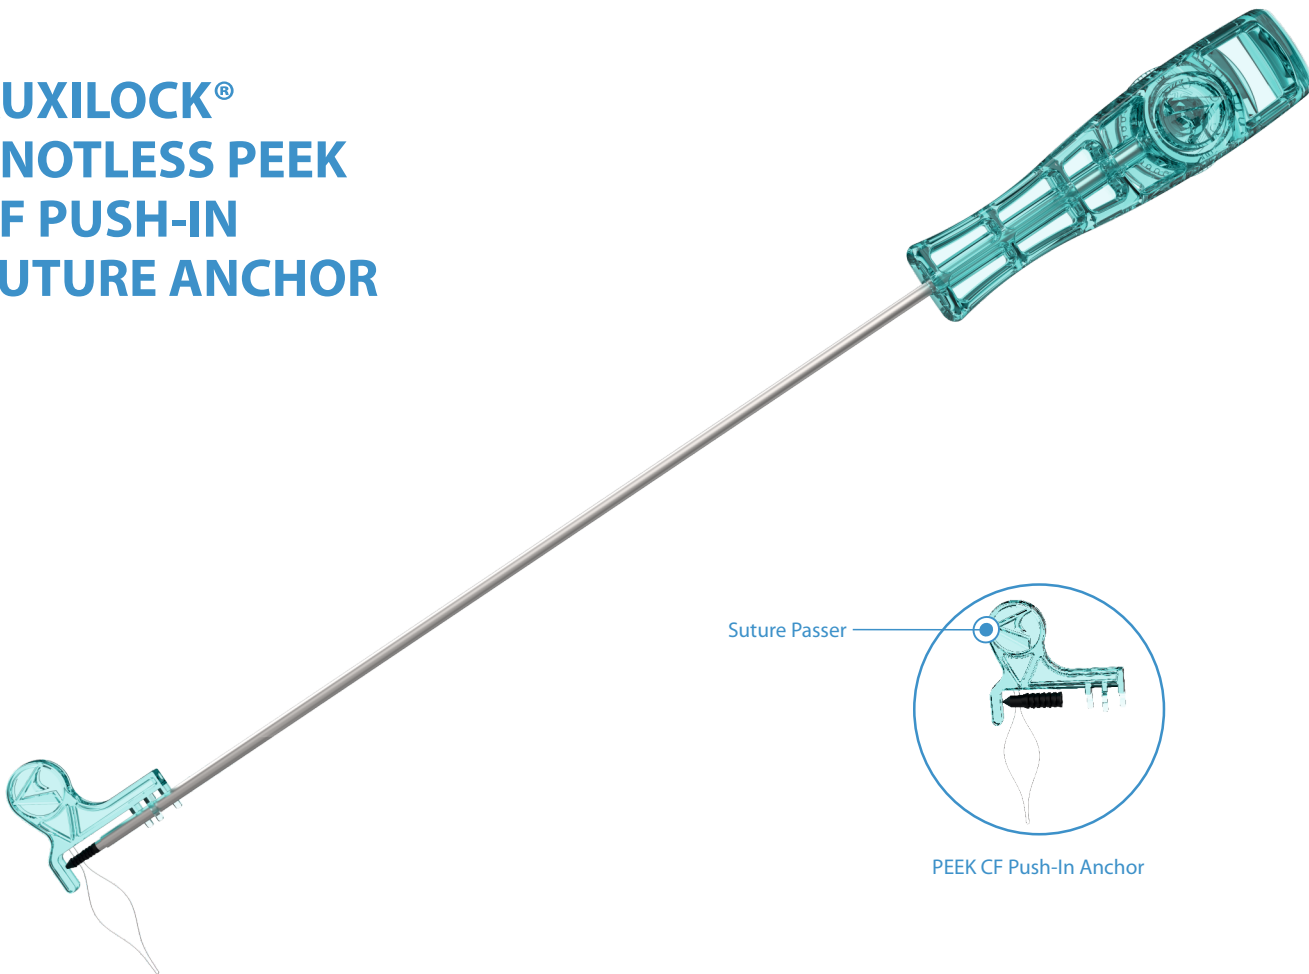

AUXILOCK[®] knotless push-in anchors are a step-saving alternative to conventional knotted suture anchors. AUXILOCK[®] knotless push-in anchors are recommended for use in Bankart and SLAP repair surgeries. These Anchors are made of carbon fiber-reinforced PEEK-OPTIMA and are available in a variety of diameters of 2.8mm and 3.5mm providing intraoperative flexibility. The PEEK CF provides modulus of elasticity closely matching the cortical bone. It is non-absorbable, radiolucent, and MRI safe. The knotless technology of Push-in anchor also eliminates knot stacks associated with soft tissue irritation.

Ordering Information

Code	Product Description
6-003-01	AUXILOCK [®] 2.8mm Knotless PEEK CF Push-In Suture Anchor With Driver, With Suture Passer
6-003-02	AUXILOCK [®] 3.5mm Knotless PEEK CF Push-In Suture Anchor With Driver, With Suture Passer


Recommended Instrumentation

Code	Product Description	Compatible Implants
7-013-01	8 Point Slotted Drill Guide, Length 190mm	6-003-01, 6-003-02
7-013-54	Ø2.5mm X 200 mm Drill Bit (For Knotless Anchor)	6-003-01
7-013-55	Ø3.2mm X 200 mm Drill Bit (For Knotless Anchor)	6-003-02
7-013-02	8 Point Drill Guide, Length 100mm	6-003-01, 6-003-02

STERILE EO

AUXILOCK[®] KNOTLESS PEEK OPTIMA PUSH-IN SUTURE ANCHOR

Shoulder Instability Repair

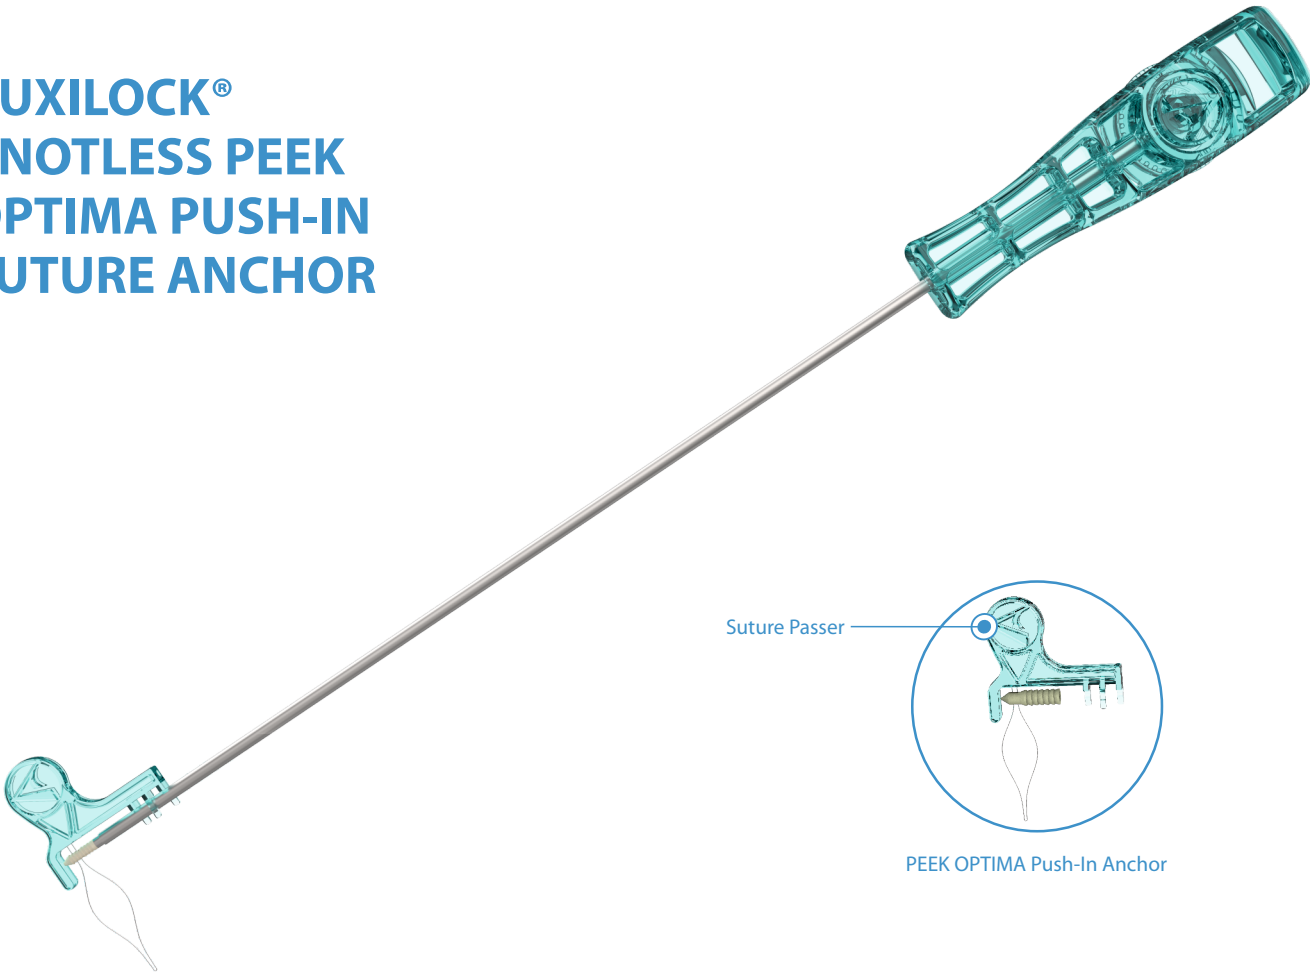

AUXILOCK[®] knotless push-in anchors are a step-saving alternative to conventional knotted suture anchors and are recommended for use in Bankart and SLAP repairs. The PEEK OPTIMA Push-In Suture Anchors are made of PEEK-OPTIMA (Poly-ether-ether-ketone). These Anchors are available in a variety of diameters of 2.8mm and 3.5mm providing intraoperative flexibility. The PEEK OPTIMA Push-In Suture Anchor is a one-piece body anchor with a material eyelet. It provides superior abrasion resistance due to PEEK's low coefficient friction. It is Biocompatible, radiolucent, and MRI safe. The knotless technology of Push-in anchor also eliminates knot stacks associated with soft tissue irritation.

Ordering Information

Code	Product Description
6-031-01	AUXILOCK [®] 2.8mm Knotless PEEK OPTIMA Push-In Suture Anchor With Driver, With Suture Passer
6-031-02	AUXILOCK [®] 3.5mm Knotless PEEK OPTIMA Push-In Suture Anchor With Driver, With Suture Passer

Recommended Instrumentation

Code	Product Description	Compatible Implants
7-013-01	8 Point Slotted Drill Guide, Length 190mm	6-031-01, 6-031-02
7-013-54	Ø2.5mm X 200 mm Drill Bit (For Knotless Anchor)	6-031-01
7-013-55	Ø3.2mm X 200 mm Drill Bit (For Knotless Anchor)	6-031-02
7-013-02	8 Point Drill Guide, Length 100mm	6-031-01, 6-031-02

STERILE EO

AUXILOCK[®]
GYROLOCK PEEK
OPTIMA KNOTLESS
SCREW IN ANCHOR



Shoulder Instability Repair

GyroLock Knotless PEEK OPTIMA Screw-in Anchors consists of PEEK-OPTIMA (Poly-ether-ether-ketone) material. The GyroLock suture anchor comes with Dual start thread technology (fast inserting suture anchor) which allows anchor deployment in 3.5 rotation.

Vented and cannulated GyroLock anchors are designed for repair and reconstruction with soft-tissue graft. GyroLock anchor is available with multiple BioBraid suture and suture tape configurations.

GyroLock suture anchor eyelet can accommodate up to four 1.4mm tapes or four #2 sutures.

Ordering Information

Code	Product Description
6-052-01	AUXILOCK [®] GyroLock 3.5mm x 15.8mm Knotless PEEK OPTIMA Screw-In Anchor


Related Instrumentation

Code	Product Description
7-013-71	Tap for 3.5mm GyroLock Screw-In Anchor

STERILE EO

AUXILOCK[®] TENDO PEEK CF SCREW-IN ANCHOR

PEEK OPTIMA Washer



PEEK CF Tendo Screw



AUXILOCK[®] Tendo PEEK CF Screw-In Anchor is ideal for proximal biceps tenodesis repair. It is available in 7.0, 8.0 and 9.0mm diameters with PEEK CF interference/tenodesis screw and PEEK OPTIMA washer. The Eyelet is specifically designed to hold the biceps tendon at the bottom of the drill hole. After fixing up the tendon into the drill hole, it can be locked into the bone by advancing the tenodesis screw. The anchor is designed to save steps and minimize the length of the procedure.

Ordering Information


Code	Product Description
6-043-01	AUXILOCK [®] Tendo 7.0mm x 15mm PEEK CF Screw-In Anchor
6-043-02	AUXILOCK [®] Tendo 8.0mm x 15mm PEEK CF Screw-In Anchor
6-043-03	AUXILOCK [®] Tendo 9.0mm x 15mm PEEK CF Screw-In Anchor
6-043-04	AUXILOCK [®] Tendo 7.0mm x 10mm PEEK CF Screw-In Anchor
6-043-05	AUXILOCK [®] Tendo 8.0mm x 10mm PEEK CF Screw-In Anchor
6-043-06	AUXILOCK [®] Tendo 9.0mm x 10mm PEEK CF Screw-In Anchor

Recommended Instrumentation

Code	Product Description
7-013-58	Graft Sizer, 6.0mm to 9.0mm (1.0mm Steps)
7-013-59	Ø6.0mm Trocar Tip Headed Reamer
7-013-60	Ø7.0mm Trocar Tip Headed Reamer
7-013-61	Ø8.0mm Trocar Tip Headed Reamer
7-013-62	Ø9.0mm Trocar Tip Headed Reamer

STERILE EO

AUXILOCK[®] TENDO PEEK OPTIMA SCREW-IN ANCHOR

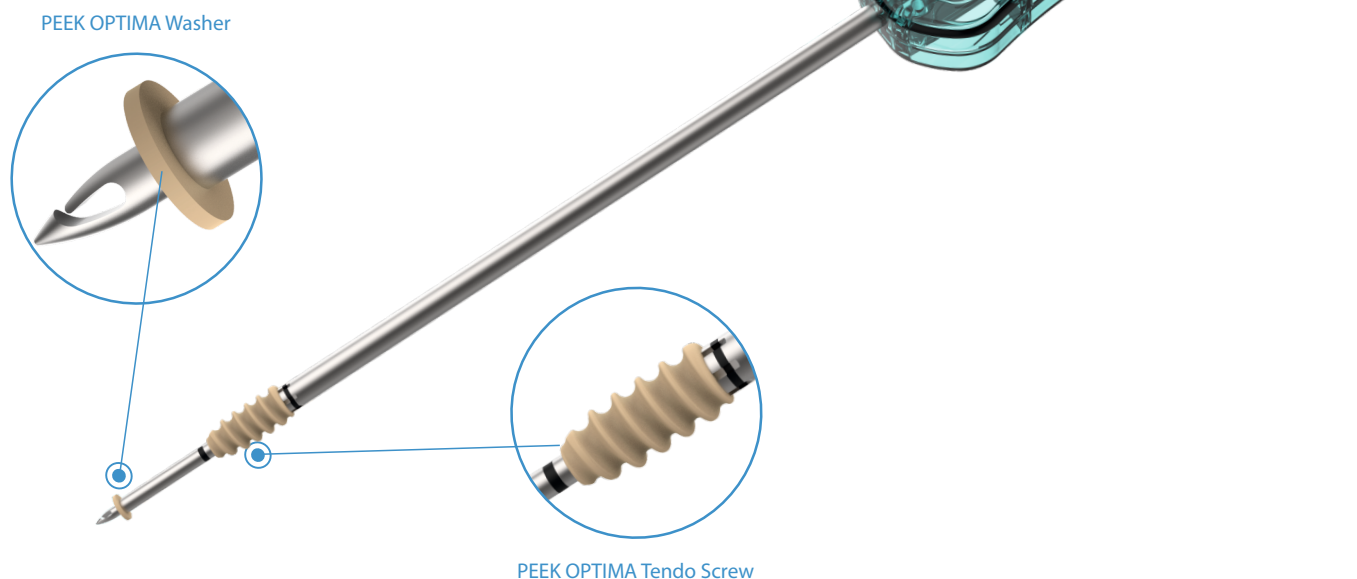

AUXILOCK[®] Tendo PEEK OPTIMA Screw-In Anchor is ideal for proximal biceps tenodesis repair. It is available in 7.0, 8.0 and 9.0mm diameters with PEEK OPTIMA interference/tenodesis screw and PEEK OPTIMA Washer. The Eyelet is specifically designed to hold the biceps tendon at the bottom of the drill hole. After fixing up the tendon into the drill hole, it can be locked into the bone by advancing the tenodesis screw. The anchor is designed to save steps and minimize the length of the procedure.

Ordering Information

Code	Product Description
6-042-01	AUXILOCK [®] Tendo 7.0mm x 15mm PEEK OPTIMA Screw-In Anchor
6-042-02	AUXILOCK [®] Tendo 8.0mm x 15mm PEEK OPTIMA Screw-In Anchor
6-042-03	AUXILOCK [®] Tendo 9.0mm x 15mm PEEK OPTIMA Screw-In Anchor
6-042-04	AUXILOCK [®] Tendo 7.0mm x 10mm PEEK OPTIMA Screw-In Anchor
6-042-05	AUXILOCK [®] Tendo 8.0mm x 10mm PEEK OPTIMA Screw-In Anchor
6-042-06	AUXILOCK [®] Tendo 9.0mm x 10mm PEEK OPTIMA Screw-In Anchor


Recommended Instrumentation

Code	Product Description
7-013-58	Graft Sizer, 6.0mm to 9.0mm (1.0mm Steps)
7-013-59	Ø6.0mm Trocar Tip Headed Reamer
7-013-60	Ø7.0mm Trocar Tip Headed Reamer
7-013-61	Ø8.0mm Trocar Tip Headed Reamer
7-013-62	Ø9.0mm Trocar Tip Headed Reamer

STERILE EO

AUXILOCK[®] AC JOINT KIT

AC Joint Repair

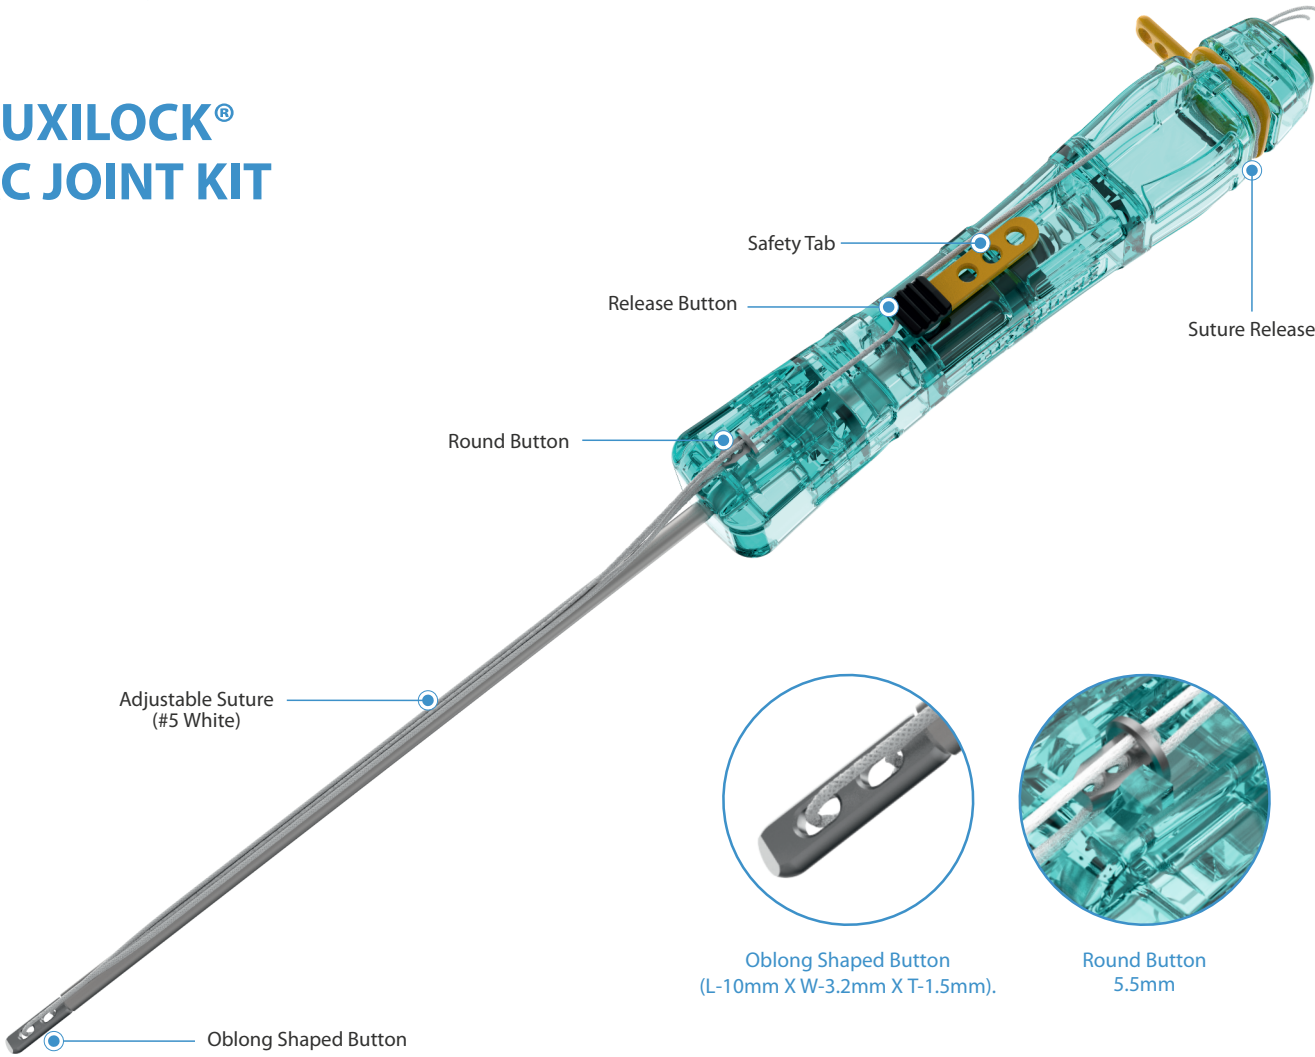

AUXILOCK[®] AC Joint Kit can be used for Acromioclavicular Joint (AC Joint) separation repair. The kit comprises of adjustable loop with round shaped button and oblong shaped button A tunnel is made through the clavicle and coracoid using 1.5mm K-Wire and 3.5mm Cannulated Drill Bit. The kit is passed through 3.5mm drilling tunnel from clavicle to coracoid provides the fixation of round button on the clavicle and oblong shaped button on the coracoid. The AC Joint Kit provides a double locking mechanism which eliminates the need for knot tying and also provides very strong compression on the clavicles.

Ordering Information

Code	Product Description
6-041-02	AUXILOCK [®] AC Joint Kit

Related Instrumentation (Include in Kit)

Code	Product Description
7-147-01	Cannulated Drill Bit with Quick Coupling End, Ø3.5mm x Length 175mm
7-147-02	Ø1.5mm K-Wire

STERILE EO

AUXILOCK[®] AUXFIX BUTTON



AC Joint Repair

AUXILOCK[®] AuxFix Button is a titanium button with holes that allow use of multiple suture tapes for AC joint reduction. It provides very strong compression on the clavicles. The button is laid on the outer surface of the clavicle or the underneath the coracoid. Only the suture material is passed through the clavicle and coracoid tunnel ensuring minimal bone loss during the procedures.

Ordering Information

Code	Product Description
6-037-01	AUXILOCK [®] AuxFix Button (AC Joint)

Related Instrumentation

Code	Product Description
7-014-68	Passing Pin Ø2.4mm X 250mm
7-013-57	Ø4.5mm Cannulated Headed Reamer

STERILE EO

7-013-01
8 Point Slotted Drill Guide, Length 190mm



7-013-02
8 Point Drill Guide, Length 100mm



7-013-03
V-Mouth Drill Guide



7-013-04
8 Point Drill Guide



7-013-05
V-Mouth Drill Guide - Curve



7-013-06
Trocar Tip Obturator



7-013-07


Trocar Tip Obturator - Curve



7-013-10

Ø1.8mm X 200mm Drill Bit

(For 2.8mm & 3.5mm Ti Needle Anchors)



7-013-11

Ø2.8mm X 200mm Drill Bit



(For 3.2mm Push-In Needle Anchor)



7-013-12

Ø2.4mm X 200mm Drill Bit


(For 2.8mm Push-In Needle Anchor)



7-013-13

Ø3.2mm X 200mm Drill Bit


(For 3.2mm AuxPix Anchor)



7-013-16

Ø1.8mm X 300mm Drill Bit


(For 2.8mm & 3.5mm Ti Anchors)



7-013-17

Ø2.4mm X 300mm Drill Bit

(For 2.8mm Push-In Anchor)




Orange



7-013-18

Ø2.8mm X 300mm Drill Bit

(For 3.5mm Push-In Anchor)




Blue



7-013-20

Ø1.5mm X 300mm Drill Bit, Stainless Steel

(For 1.5mm & 1.8mm AuxSuture Anchor)



Brown



7-013-21

Ø1.5mm X 300mm Drill Bit, Nitinol

(For 1.5mm & 1.8mm AuxSuture Anchor - Curve)



7-013-53

Ø1.8mm X 325 mm Drill Bit

(For 1.8mm AuxPix Anchor)




Golden



7-013-54

Ø2.5mm X 200 mm Drill Bit (For Knotless Anchor)


(For 2.8mm Knotless Anchor)




Pink



7-013-55
Ø3.2mm X 200 mm Drill Bit (For Knotless Anchor)
(For 3.5mm Knotless Anchor)



7-013-33
Switching Stick



7-013-22
Ø2.9mm Awl
(For 2.9mm AuxSuture Anchor)



7-013-23
Ø3.2mm Awl
(For 3.2mm AuxPix Anchor & 4.5mm Knotless Anchor)



7-013-24
Ø4.1mm Awl
(For Rotador & 5.5mm Knotless Anchor)



7-013-25
Awl For 4.5/5.5mm PEEK Screw-In Anchor
(For PEEK Screw-In Anchor)



7-013-26

Awl For 6.5mm PEEK Screw-In Anchor
(For PEEK Screw-In Anchor)



7-013-27

Awl/ Tap For 4.5/5.5mm PEEK Screw-In Anchor
(For PEEK Screw-In Anchor)



7-013-28

Awl/ Tap For 6.5mm PEEK Screw-In Anchor
(For PEEK Screw-In Anchor)



7-013-29

Tap For 4.5/5.5mm PEEK Screw-In Anchor
(For PEEK Screw-In Anchor)



7-013-30

Tap For 6.5mm PEEK Screw-In Anchor
(For PEEK Screw-In Anchor)



7-013-32

4.5/5.5mm Knotless PEEK Anchor Driver



7-013-34
Arthroscopic Probe - Shoulder



7-013-35
Tissue Elevator, 15° Up



7-013-36
Tissue Elevator, 15° Down



7-013-37
Rasp, 15° Up



7-013-38
Rasp, 15° Down




7-013-39
Ring Curette



7-013-40
Knot Pusher



7-013-44
Hammer

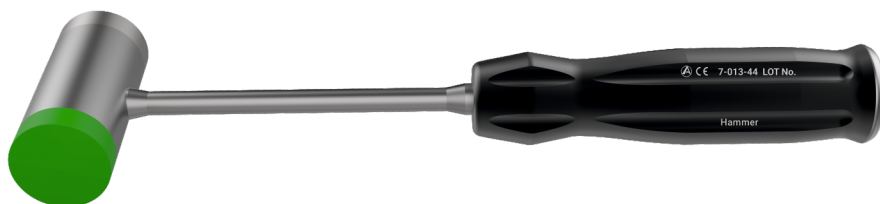

7-013-57
Ø4.5mm Cannulated Headed Reamer



7-013-58
Graft Sizer, 6.0mm to 9.0mm (1.0mm Steps)



Tocar Tip Headed Reamer



Code	Diameter
7-013-59	Ø6.0mm Tocar Tip Headed Reamer
7-013-60	Ø7.0mm Tocar Tip Headed Reamer
7-013-61	Ø8.0mm Tocar Tip Headed Reamer
7-013-62	Ø9.0mm Tocar Tip Headed Reamer

7-014-68
Passing Pin, Ø2.4mm x 250mm



7-013-69

Awl/Tap for 4.75/5.5mm Gyrolock Screw-In Anchor



7-013-70

Tap for 4.75/5.5mm Gyrolock Screw-In Anchor



7-013-71

Tap for 3.5mm Gyrolock Screw-In Anchor



OPTIONAL INSTRUMENTS


7-013-63

Tissue Elevator, 30° Up



7-013-64


Tissue Elevator, 30° Down

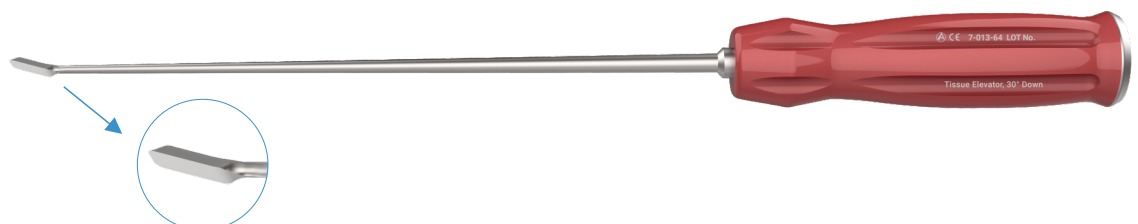

7-013-41
Suture Retriever




7-013-42
Tissue Grasper

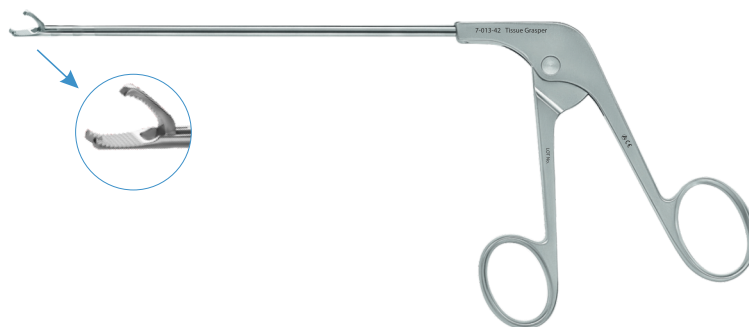

7-013-43
Suture Cutter/Knot Pusher With
Lock, Ø4.2mm, V-Knotch,
Left Opened



7-013-47
ESCORPIAN Suture Passer

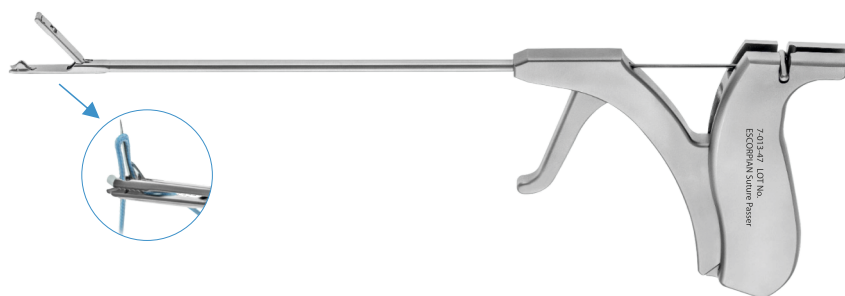


7-013-48
Needle With Lateral Opening For ESCORPIAN Suture Passer



OPTIONAL INSTRUMENTS

Smart Hook Suture passer

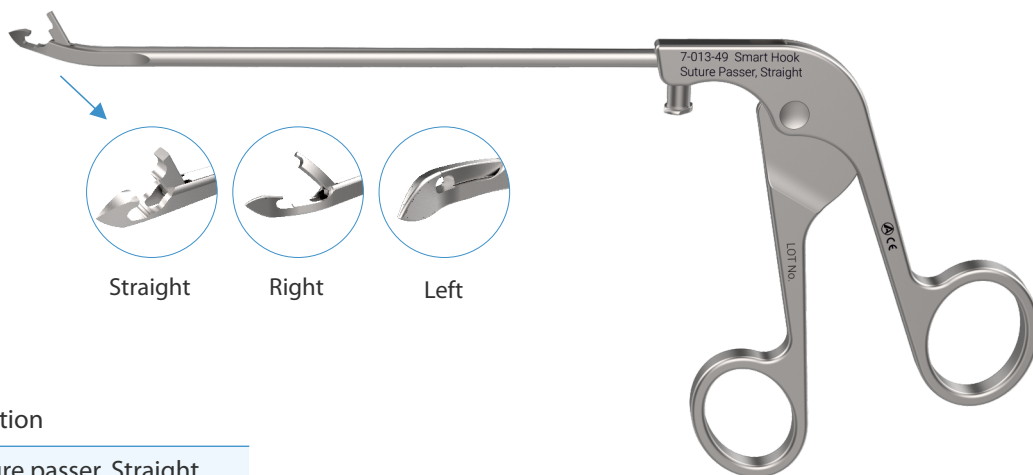

Code	Product Description
7-013-49	Smart Hook Suture passer, Straight
7-013-50	Smart Hook Suture passer, Right
7-013-51	Smart Hook Suture passer, Left


ORDER INFORMATION

7-013 **Shoulder Arthroscopy Instrument Set**

Code	Set Consisting of	Unit
7-013-01	8 Point Slotted Drill Guide, Length 190mm	1
7-013-02	8 Point Drill Guide, Length 100mm	1
7-013-03	V-Mouth Drill Guide	1
7-013-04	8 Point Drill Guide	1
7-013-05	V-Mouth Drill Guide - Curve	1
7-013-06	Trocar Tip Obturator	1
7-013-07	Trocar Tip Obturator - Curve	1
7-013-10	Ø1.8mm X 200mm Drill Bit	1
7-013-11	Ø2.8mm X 200mm Drill Bit	1
7-013-12	Ø2.4mm X 200mm Drill Bit	1
7-013-13	Ø3.2mm X 200mm Drill Bit	1
7-013-16	Ø1.8mm X 300mm Drill Bit	1
7-013-17	Ø2.4mm X 300mm Drill Bit	1
7-013-18	Ø2.8mm X 300mm Drill Bit	1
7-013-20	Ø1.5mm X 300mm Drill Bit, Stainless Steel	1
7-013-21	Ø1.5mm X 300mm Drill Bit, Nitinol	1
7-013-22	Ø2.9mm Awl	1
7-013-23	Ø3.2mm Awl	1
7-013-24	Ø4.1mm Awl	1
7-013-25	Awl For 4.5/5.5mm PEEK Screw-In Anchor	1
7-013-26	Awl For 6.5mm PEEK Screw-In Anchor	1
7-013-27	Awl/ Tap For 4.5/5.5mm PEEK Screw-In Anchor	1
7-013-28	Awl/ Tap For 6.5mm PEEK Screw-In Anchor	1
7-013-29	Tap For 4.5/5.5mm PEEK Screw-In Anchor	1
7-013-30	Tap For 6.5mm PEEK Screw-In Anchor	1
7-013-32	4.5/5.5mm Knotless PEEK Anchor Driver	1
7-013-33	Switching Stick	1
7-013-34	Arthroscopic Probe - Shoulder	1
7-013-35	Tissue Elevator, 15° Up	1
7-013-36	Tissue Elevator, 15° Down	1
7-013-37	Rasp, 15° Up	1
7-013-38	Rasp, 15° Down	1
7-013-39	Ring Curette	1
7-013-40	Knot Pusher	1
7-013-44	Hammer	1
7-013-53	Ø1.8mm X 325 mm Drill Bit	1
7-013-54	Ø2.5mm X 200 mm Drill Bit (For Knotless Anchor)	1
7-013-55	Ø3.2mm X 200 mm Drill Bit (For Knotless Anchor)	1
7-014-68	Passing Pin, Ø2.4mm x 250mm	1
7-013-57	Ø4.5mm Cannulated Headed Reamer	1

Code	Set Consisting of	Unit
7-013-58	Graft Sizer, 6.0mm to 9.0mm (1.0mm Steps)	1
7-013-59	Ø6.0mm Trocar Tip Headed Reamer	1
7-013-60	Ø7.0mm Trocar Tip Headed Reamer	1
7-013-61	Ø8.0mm Trocar Tip Headed Reamer	1
7-013-62	Ø9.0mm Trocar Tip Headed Reamer	1
7-013-69	Awl/Tap for 4.75/5.5mm Gyrolock Screw-In Anchor	1
7-013-70	Tap for 4.75/5.5mm Gyrolock Screw-In Anchor	1
7-013-71	Tap for 3.5mm Gyrolock Screw-In Anchor	1
7-013-66	Instrument Tray A for Shoulder Arthroscopy Instrument Set	1
7-013-67	Instrument Tray B for Shoulder Arthroscopy Instrument Set	1
7-013-68	Instrument Tray C for Shoulder Arthroscopy Instrument Set	1
7-013-46	Container For Shoulder Arthroscopy Instrument Set	1
7-013-52	Lid For Container Shoulder Arthroscopy Instrument Set	1


7-013-66
Instrument Tray A for Shoulder Arthroscopy Instrument set

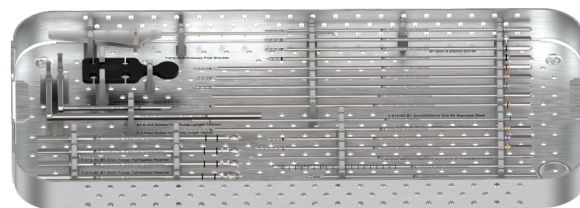

7-013-67
Instrument Tray B for Shoulder Arthroscopy Instrument set




7-013-68
Instrument Tray C for Shoulder Arthroscopy Instrument set

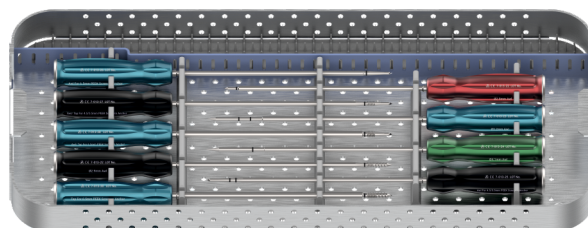

7-013-46
Container For Shoulder Arthroscopy Instrument Set



7-013-52
Lid For Container Shoulder Arthroscopy Instrument Set

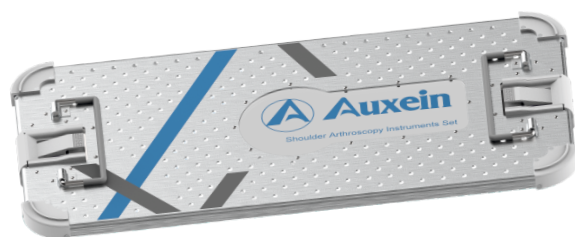

OPTIONAL INSTRUMENTS

7-013-41	Suture Retriever	1
7-013-42	Tissue Grasper	1
7-013-43	Suture Cutter/Knot Pusher With Lock, Ø4.2mm, V-Knotch, Left Opened	1
7-013-47	ESCORPIAN Suture Passer	1
7-013-48	Needle With Lateral Opening For ESCORPIAN Suture Passer	1
7-013-49	Smart Hook Suture passer, Straight	1
7-013-50	Smart Hook Suture passer, Right	1
7-013-51	Smart Hook Suture passer, Left	1
7-013-63	Tissue Elevator, 30° Up	1
7-013-64	Tissue Elevator, 30° Down	1



USA

Auxein Inc.

1500 Nw 89th Court, Suite 107-108
Doral, Florida 33172

Tel: +1 305 395 6062

E Fax: +1 305 395 6262

Email: USoffice@auxein.com

MEXICO

Auxein México, S.A. de C.V.

Tepic 139 int 801, Colonia Roma Sur,
Alcaldía Cuauhtémoc, CDMX,
México, C.P. 06760

Tel: +521 55 7261 0318

Email: info@auxein.mx

INDIA

Auxein Medical Pvt. Ltd.

Plot No. 168-169-170, Phase-4,
Kundli Industrial Area,
HSIIDC, Sector-57, Sonapat - 131028, Haryana

Tel: +91 99106 43638 | Fax: +91 86077 70197

Email: info@auxein.com

www.auxein.com