


Austin Moore Hip Prosthesis, Standard Stem



Fig: Test Setup

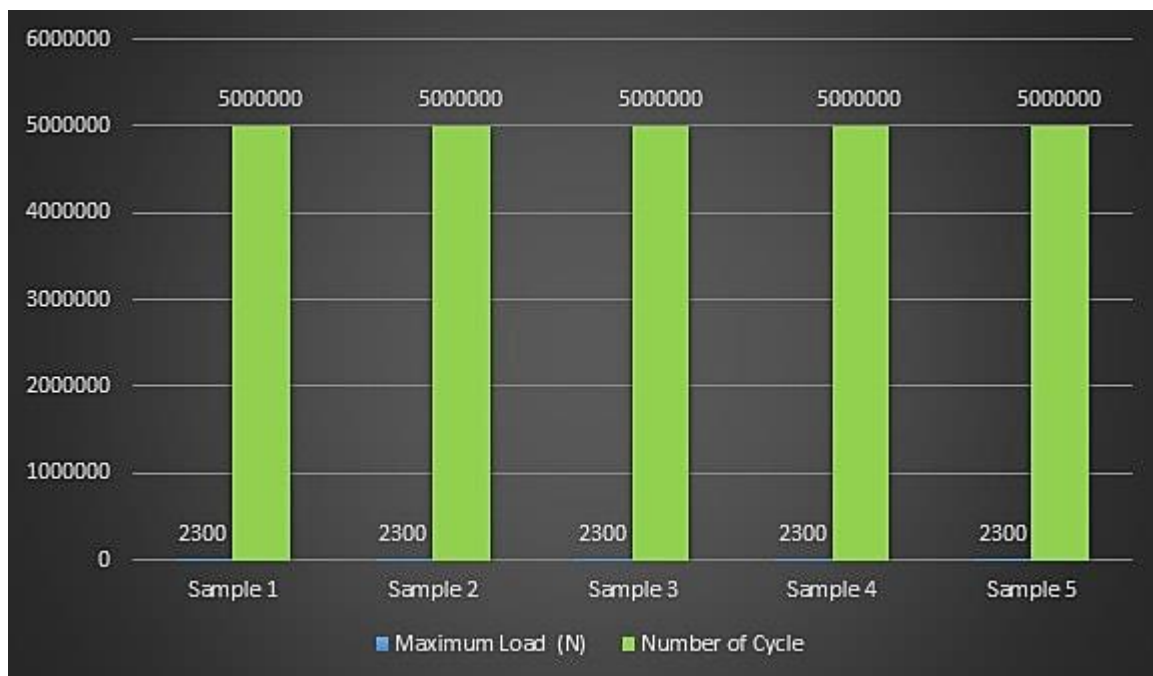

The Metallic Hip Prosthesis Manufactured by M/S Auxein Medical Pvt. Ltd. tested as per the test method described in ISO 7206-4 “Determination of endurance properties and performance of stemmed femoral components.”