



**JIN Type Humerus Nail, Dia. 6mm X Length 320mm, Titanium**



*Fig: Test Setup*

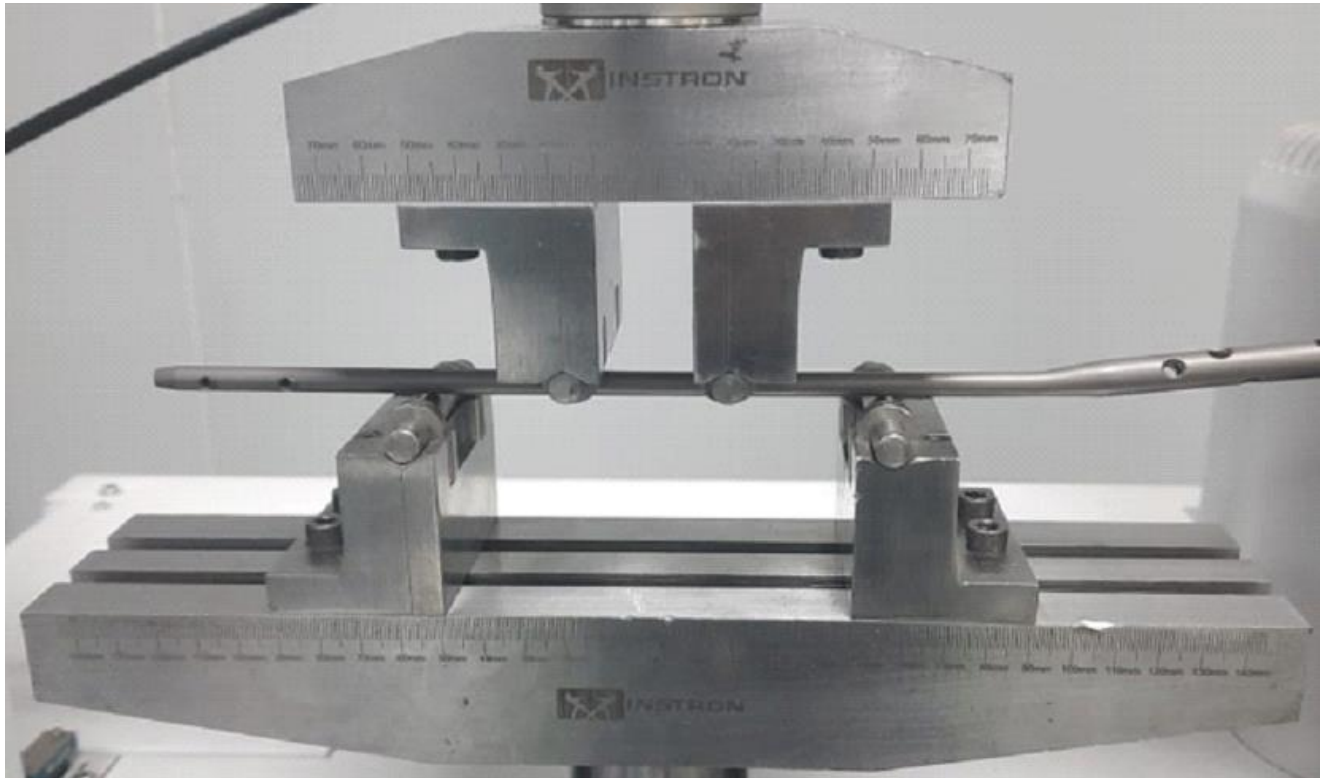

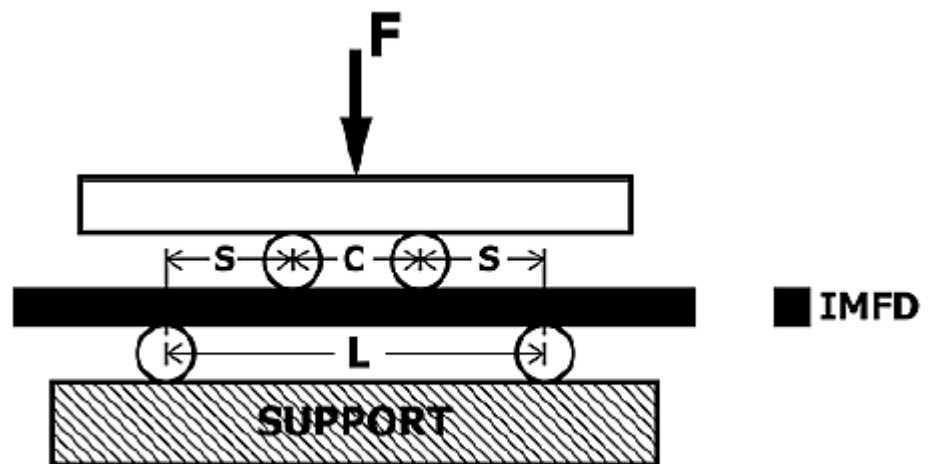



JIN TYPE Humerus Nail Manufactured by M/S Auxein Medical Pvt. Ltd. tested as per the test method described in ASTM F1264 for four point bend testing in order to determine the Yield load (N) as well as bending strength under the flexural loading.