

PALLAS-Low Profile Anterior Cervical Fusion Device, Convex, Standard, 12mm, Titanium


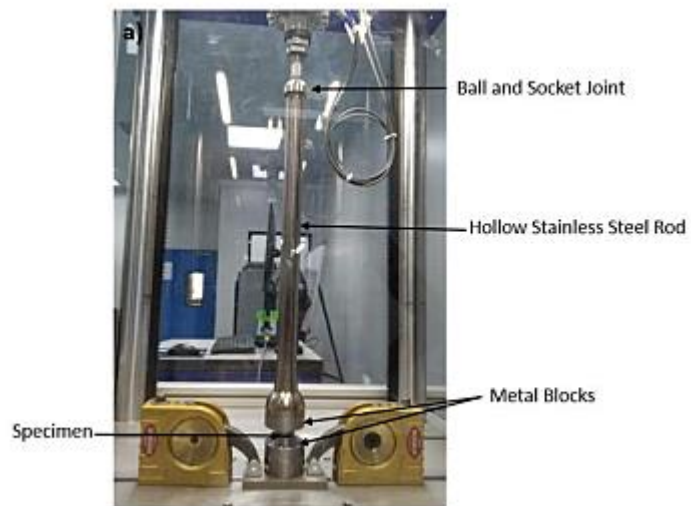


Fig: Test Setup

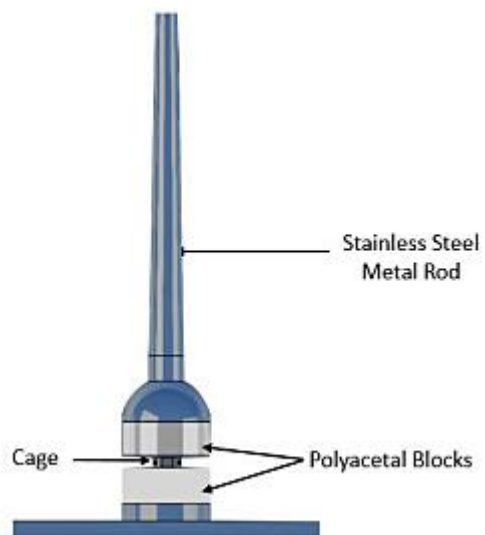

The spinal cages Manufactured by M/S Auxein Medical Pvt. Ltd. tested as per the test method described in ASTM F2077.