
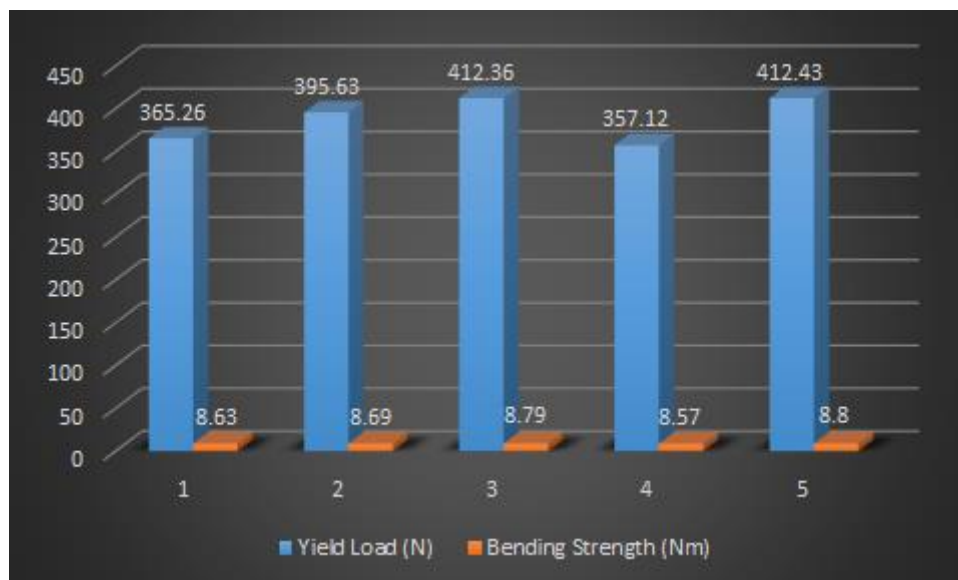


PHEELOS-3.5mm Small Fragments, Titanium

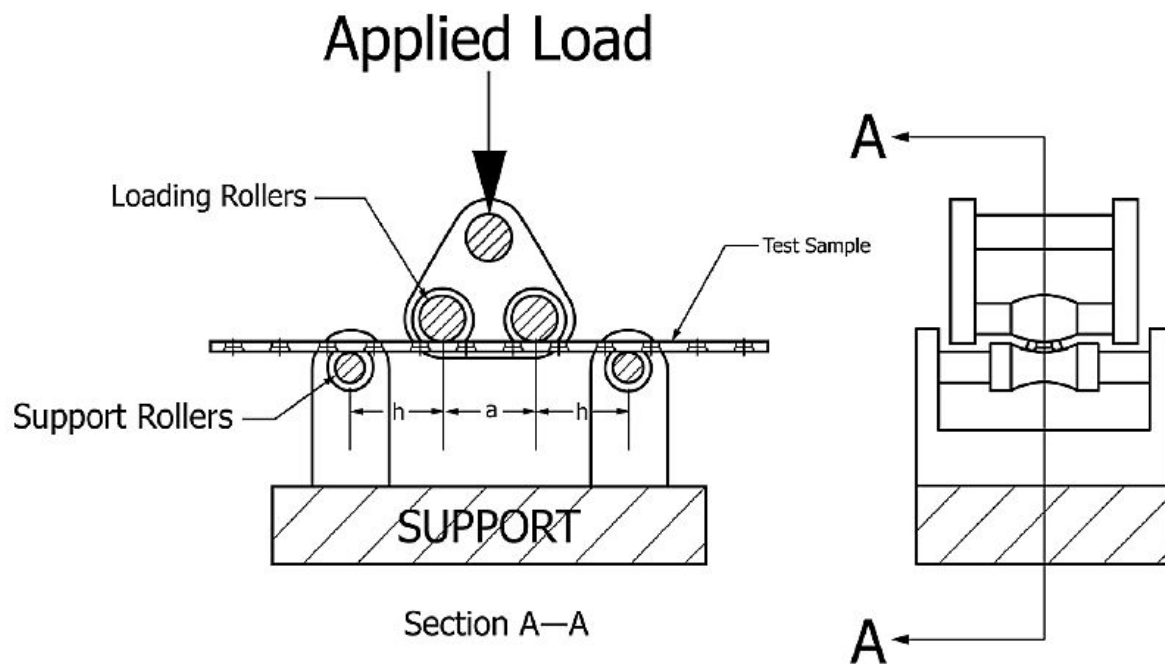

The Metallic Bone plates Manufactured by M/S Auxein Medical Pvt. Ltd. tested as per the test method described in ASTM F382-17 for four point bend testing in order to determine the Yield load (N) as well as bending strength under the flexural loading.