

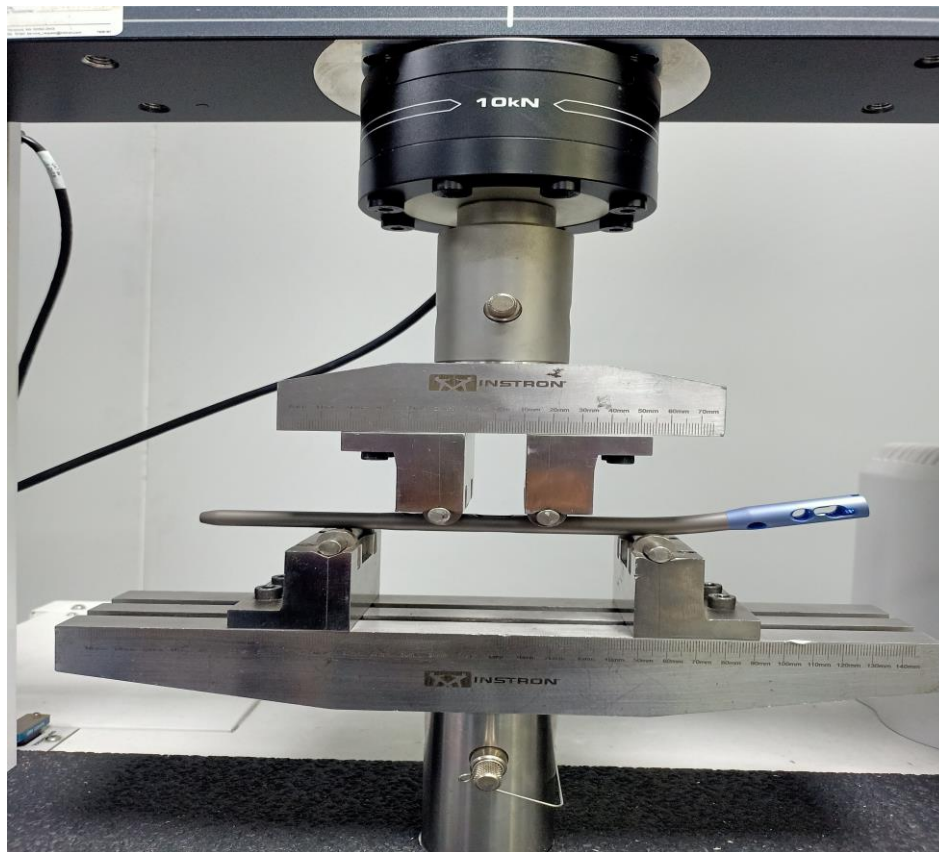


Tarsus Nail, dia. 10mm and length 240mm, Titanium



*Fig: Test Setup*

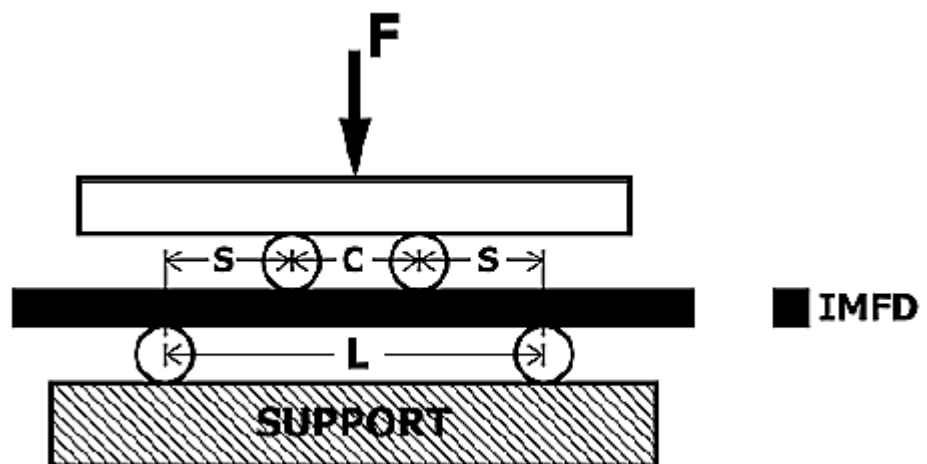

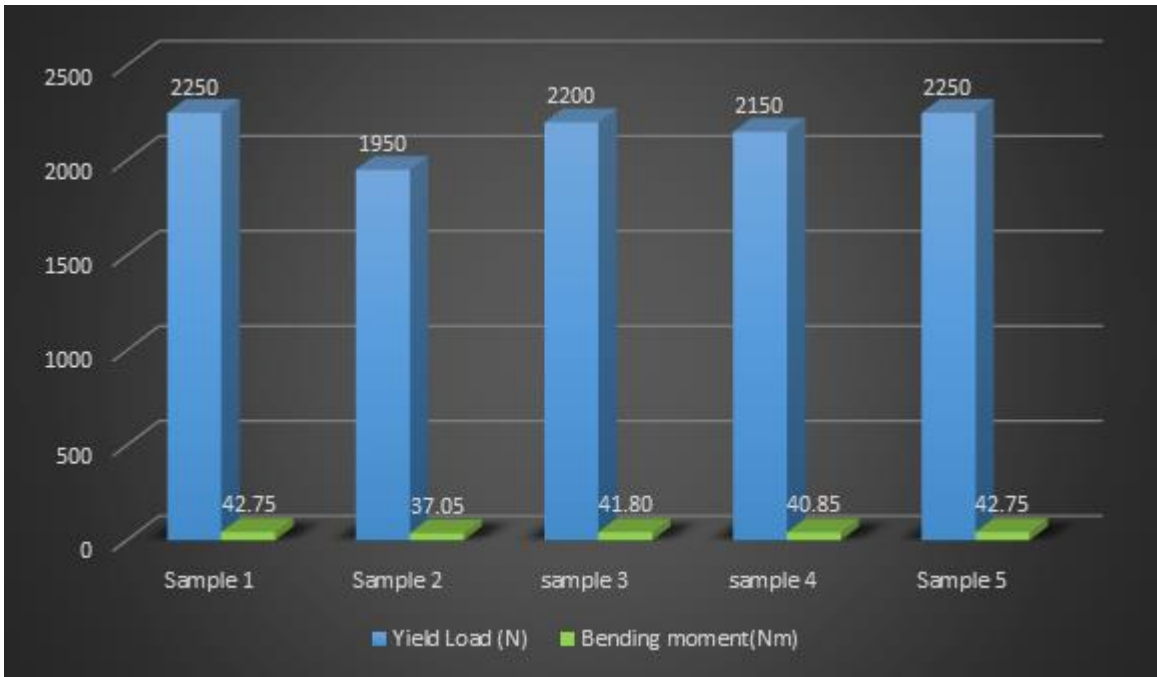

The Tarsus Nail Manufactured by M/S Auxein Medical Pvt. Ltd. tested as per the test method described in ASTM F1264 for four point bend testing in order to determine the Yield load (N) as well as bending strength under the flexural loading.