


VERTAUX - Occipital Poly axial Pedicle Screw, Partial Thread, Ø4.0mm x Length 40mm, Titanium

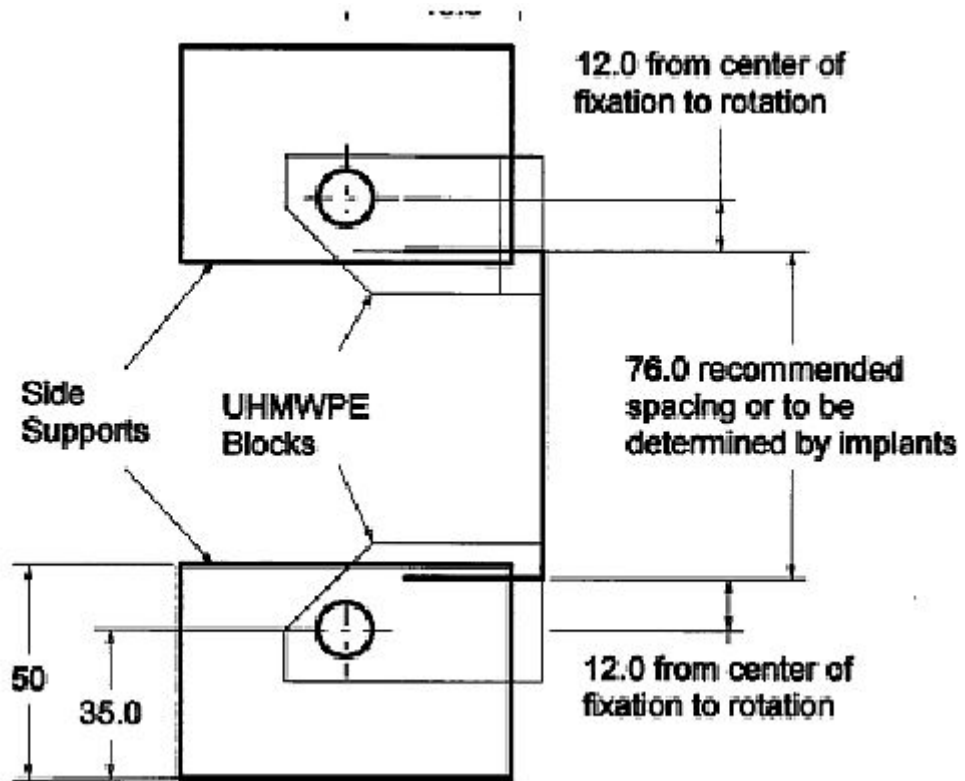

This test series was conducted to determine the torsional performance of Spinal System devices including hybrid construct of Auxein Medical as per ASTM F1717.