


AUXILOCK® AUXSUTURE ANCHOR

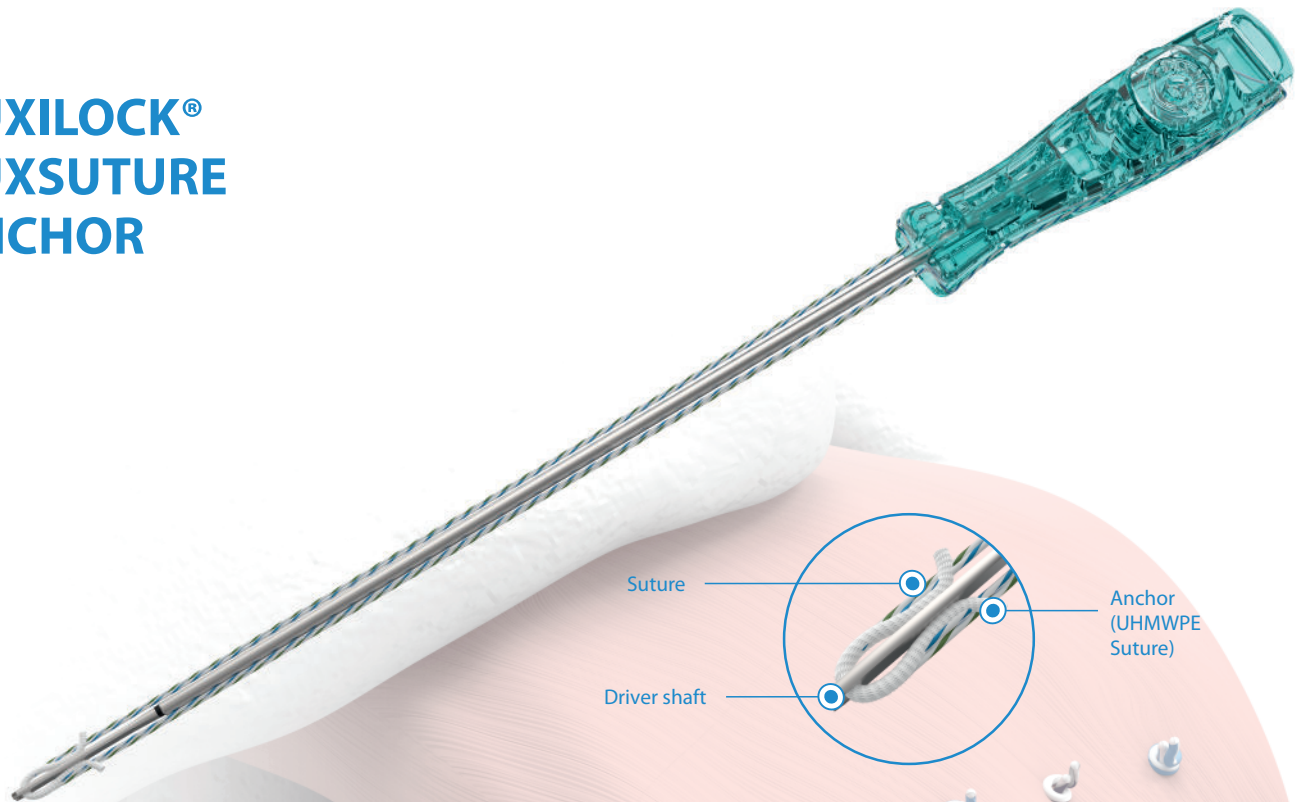

Rotator Cuff Repair

AUXILOCK® AuxSuture Anchor provides numerous advantages over traditional anchors. The strong fixation, less bone removal and a push in technique provide higher efficiency in rotator cuff repair procedures. AuxSuture anchor is available in diameter of 2.9mm. It requires a pilot hole for its insertion. The specially designed 2.9mm Awl for AuxSuture Anchor provides an accurate hole placement for the anchor. The small 2.9mm footprint of AuxSuture anchor provides placement and fixation advantages when bone real estate is limited, especially during revision surgeries. AuxSuture Anchor is available in double and triple loaded options with various combination of BioBraid and suture tapes.

Ordering Information

Code	Product Description	Suture/Tape Colour	Needle
6-036-01	AUXILOCK® 2.9mm AuxSuture Anchor With Two #2 BioBraid: White/Blue & White/Green		
6-036-02	AUXILOCK® 2.9mm AuxSuture Anchor With Two #2 BioBraid: White/Blue & White/Green, With Needle: MO-6		
6-036-03	AUXILOCK® 2.9mm AuxSuture Anchor With Three #2 BioBraid: White, White/Blue & White/Green		
6-036-04	AUXILOCK® 2.9mm AuxSuture Anchor With One #2 BioBraid and One 1.4mm Suture Tape: White/Black & White/Blue		
6-036-05	AUXILOCK® 2.9mm AuxSuture Anchor With Two 1.4mm Suture Tape: White/Black & White/Blue		

Recommended Instrumentation

Code	Product Description	Compatible Implants
7-013-22	Ø2.9mm Awl	6-036-01, 6-036-02, 6-036-03, 6-036-04, 6-036-05

STERILE|EO