


AUXILOCK[®] KNOTLESS PEEK OPTIMA PUSH-IN SUTURE ANCHOR

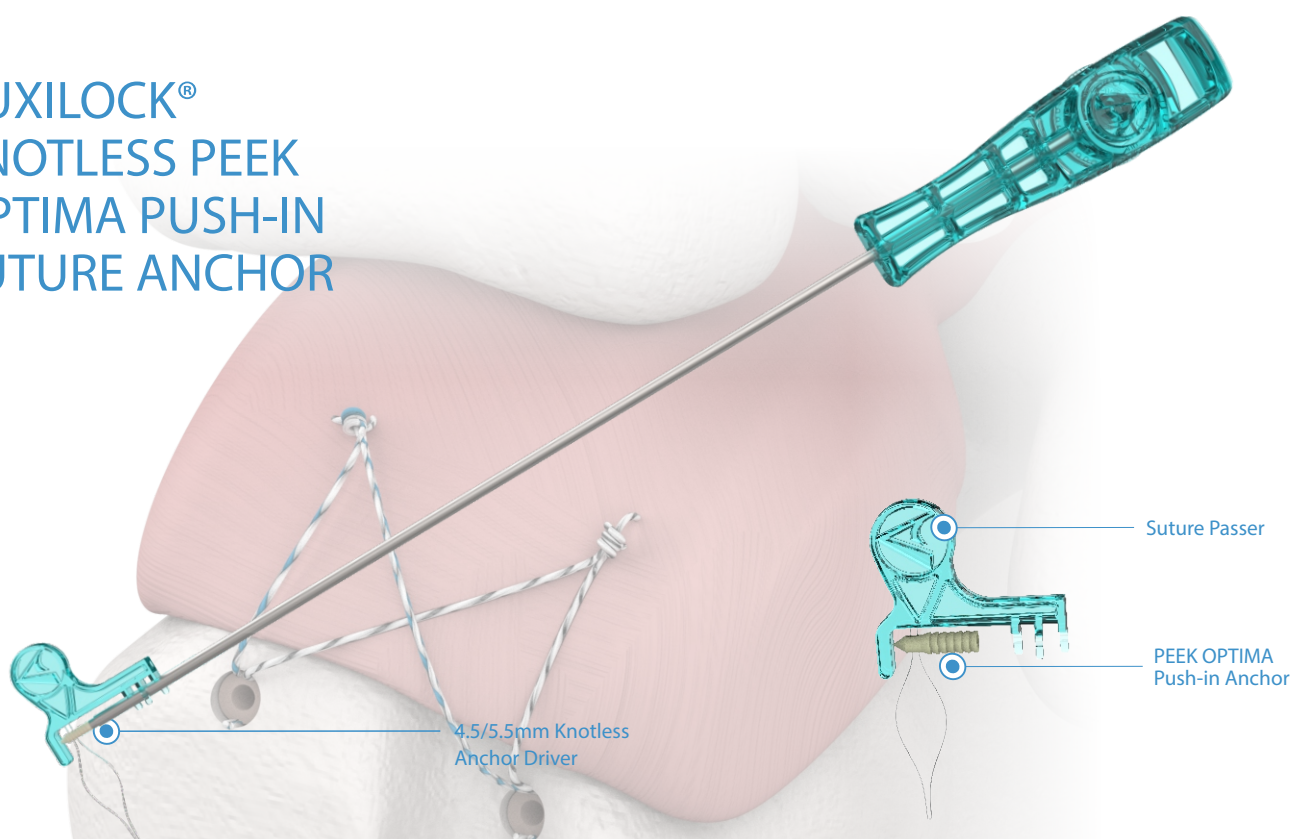

AUXILOCK[®] knotless push-in anchors provide a step-saving alternative to conventional knotted suture anchors. AUXILOCK[®] knotless push-in anchors are recommended for use in both large and small-joint soft tissue repairs. PEEK OPTIMA Push-In Suture Anchors consists of PEEK-OPTIMA (Poly-ether-ether-ketone) and are available in a variety of diameters of 4.5mm and 5.5mm providing intraoperative flexibility. The PEEK OPTIMA Push-In Suture Anchor is a non-absorbable PEEK suture anchor with a eyelet. Hence, providing superior abrasion resistance due to PEEK's low coefficient friction. It is biocompatible, radiolucent, and MRI safe. The knotless technology of Push-in anchor also eliminates knot stacks associated with soft tissue irritation. The anchor is available with and without driver. The 4.5/5.5mm knotless anchor driver is provided separately in the instrument set. It is reusable driver that minimizes the cost of the surgery unlike the pre-loaded suture anchors.

Ordering Information

Code	Product Description
6-031-04	AUXILOCK [®] 4.5mm Knotless PEEK OPTIMA Push-In Suture Anchor With Suture Passer
6-031-05	AUXILOCK [®] 5.5mm Knotless PEEK OPTIMA Push-In Suture Anchor With Suture Passer
6-031-07	AUXILOCK [®] 4.5mm Knotless PEEK OPTIMA Push In Suture Anchor With Driver, With Suture Passer
6-031-08	AUXILOCK [®] 5.5mm Knotless PEEK OPTIMA Push In Suture Anchor With Driver, With Suture Passer

Recommended Instrumentation

Code	Product Description	Compatible Implants
7-013-23	Ø3.2mm Awl	6-031-04, 6-031-07
7-013-24	Ø4.1mm Awl	6-031-05, 6-031-08
7-013-32	4.5/5.5mm Knotless PEEK Anchor Driver	6-031-04, 6-031-05

STERILE EO